

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121317\
 Data File : BM013378.D
 Acq On : 13 Dec 2017 17:48
 Operator : SJ/JU
 Sample : PB104973BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 14 01:19:55 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 14 01:15:39 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	93389	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	410743	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.33	164	271300	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	756270	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	1015046	20.00	ng/ul	0.00
83) Perylene-d12	23.49	264	936811	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	11842	6.28	ng/uL	0.00
5) Phenol-d5	6.86	99	217531	26.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	128835	27.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	176926	28.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	181803	26.34	ng/ul	0.00
19) Nitrobenzene-d5	8.84	128	96396	29.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	99527	28.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	195235	27.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	275826	41.78	ng/ul	0.00
43) Dimethylphthalate-d6	13.74	166	722706	29.94	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	886241	29.75	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	115201	27.46	ng/ul	0.00
57) Fluorene-d10	15.32	176	655042	31.55	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	93693	19.69	ng/ul	0.00
70) Anthracene-d10	17.17	188	1227137	32.40	ng/ul	0.00
76) Pyrene-d10	19.47	212	1570533	31.06	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.35	264	1584200	33.20	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.39	70	5934	1.122	ng/ul# 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121317\
Data File : BM013378.D
Acq On : 13 Dec 2017 17:48
Operator : SJ/JU
Sample : PB104973BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Dec 14 01:19:55 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 14 01:15:39 2017
Response via : Initial Calibration

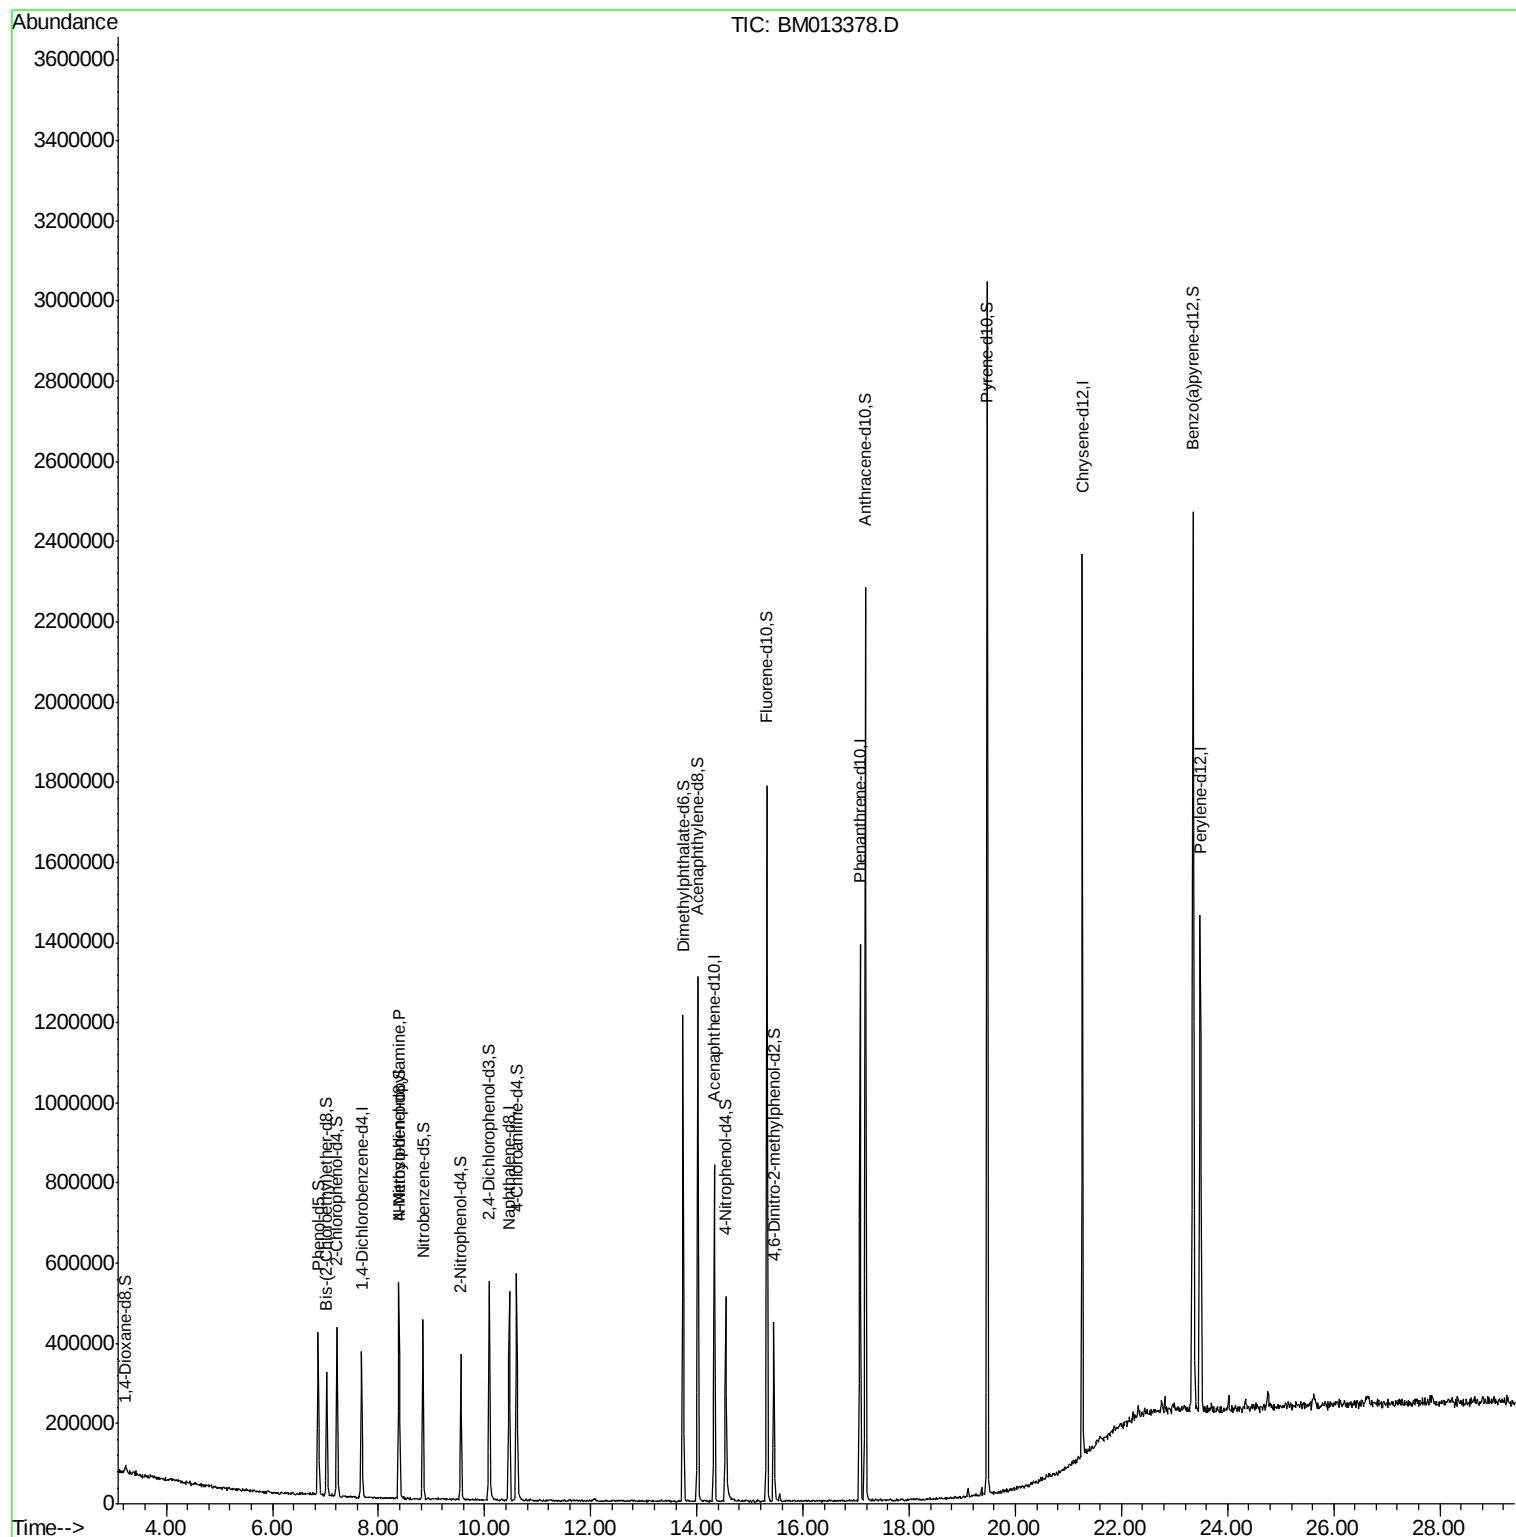

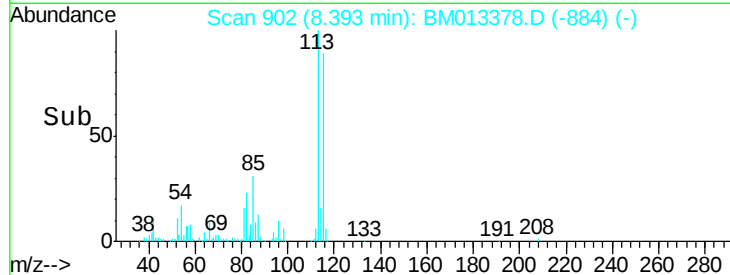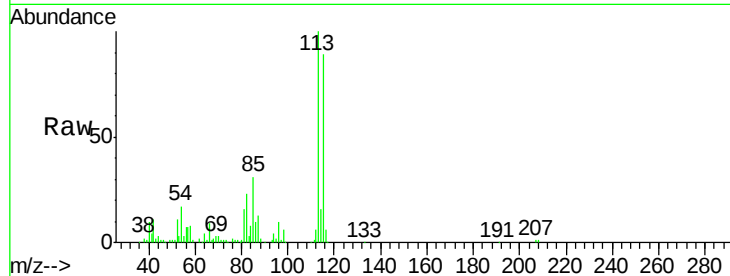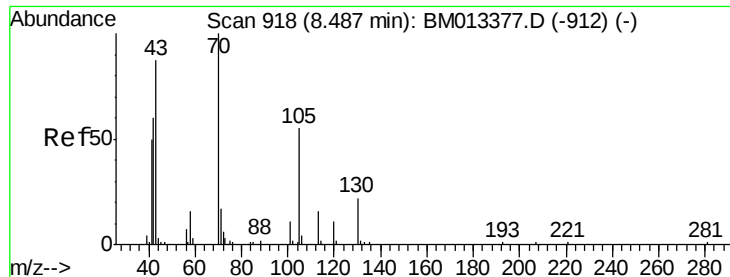

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.122 ng/ul
 RT: 8.39 min Scan# 902
 Delta R.T. -0.09 min
 Lab File: BM013378.D
 Acq: 13 Dec 2017 17:48

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:	70	Resp:	5934
Ion	Ratio	Lower	Upper
70	100		
42	330.3	76.0	114.0#
101	0.0	6.7	10.1#
130	0.0	14.6	22.0#

