

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048974.D
 Acq On : 13 Dec 2024 09:45
 Operator : RC/JU
 Sample : PB165168BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK168

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	25	28	36	rVB	76925	97853	2.98%	0.255%
2	3.546	91	95	108	rBV	919611	1287515	39.27%	3.357%
3	3.858	144	148	153	rBV	23015	32373	0.99%	0.084%
4	4.069	182	184	191	rVB6	9675	14254	0.43%	0.037%
5	4.158	197	199	202	rBV3	3936	3735	0.11%	0.010%
6	4.287	219	221	224	rBV4	4396	4598	0.14%	0.012%
7	4.381	235	237	243	rVB5	3189	4251	0.13%	0.011%
8	4.469	250	252	258	rVB4	7386	7780	0.24%	0.020%
9	4.928	327	330	335	rVB5	2845	5410	0.16%	0.014%
10	6.416	580	583	585	rBV4	3903	4368	0.13%	0.011%
11	6.463	588	591	594	rBV5	2795	3336	0.10%	0.009%
12	6.757	634	641	655	rBV	897204	1392519	42.47%	3.631%
13	6.916	662	668	679	rVB	774053	1180602	36.01%	3.078%
14	7.110	694	701	713	rBV	908244	1386486	42.29%	3.615%
15	7.569	772	779	789	rVB	688412	1075349	32.80%	2.804%
16	7.675	795	797	801	rBV4	2356	3295	0.10%	0.009%
17	8.275	892	899	913	rBV	989659	1545656	47.14%	4.030%
18	8.710	967	973	983	rBV	757053	1241346	37.86%	3.236%
19	9.428	1088	1095	1105	rBV	506934	813938	24.82%	2.122%
20	9.963	1178	1186	1200	rBV	872502	1428958	43.58%	3.726%
21	10.334	1242	1249	1258	rVB	843255	1386145	42.28%	3.614%
22	10.475	1266	1273	1285	rBV	853236	1455454	44.39%	3.795%
23	11.528	1451	1452	1455	rBV3	3228	3376	0.10%	0.009%
24	11.939	1517	1522	1526	rBV5	8544	14374	0.44%	0.037%
25	13.628	1801	1809	1821	rBV	1383821	1880435	57.35%	4.903%
26	13.898	1848	1855	1865	rBV	1652443	2420522	73.82%	6.311%
27	14.204	1900	1907	1918	rBV	1085958	1570222	47.89%	4.094%
28	14.410	1936	1942	1962	rBV	460059	758008	23.12%	1.976%
29	14.539	1962	1964	1968	rVB4	3670	3681	0.11%	0.010%
30	14.628	1976	1979	1982	rVB4	3415	4305	0.13%	0.011%
31	15.204	2070	2077	2085	rBV	2145062	2854467	87.06%	7.442%
32	15.322	2091	2097	2110	rBV	403418	554241	16.90%	1.445%
33	15.445	2114	2118	2124	rVB5	10605	16753	0.51%	0.044%
34	15.992	2207	2211	2214	rBV6	4169	5892	0.18%	0.015%
35	16.951	2368	2374	2384	rBV	1235526	1650065	50.32%	4.302%
36	17.051	2384	2391	2403	rBV	2197755	2939268	89.64%	7.663%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048974.D
Acq On : 13 Dec 2024 09:45
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK168

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Title : SVOA CALIBRATION

37	18.745	2677	2679	2682	rBV3	2929	3494	0.11%	0.009%
38	18.916	2704	2708	2714	rBV4	21009	26967	0.82%	0.070%
39	18.986	2716	2720	2726	rVV3	16859	23115	0.70%	0.060%
40	19.351	2775	2782	2796	rBV	2657494	3278842	100.00%	8.548%
41	21.174	3087	3092	3100	rBV	1136953	1502738	45.83%	3.918%
42	23.792	3529	3537	3548	rBV	1361759	2923738	89.17%	7.623%
43	23.980	3562	3569	3578	rBV2	698349	1546222	47.16%	4.031%




Sum of corrected areas: 38355946

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048974.D
Acq On : 13 Dec 2024 09:45
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

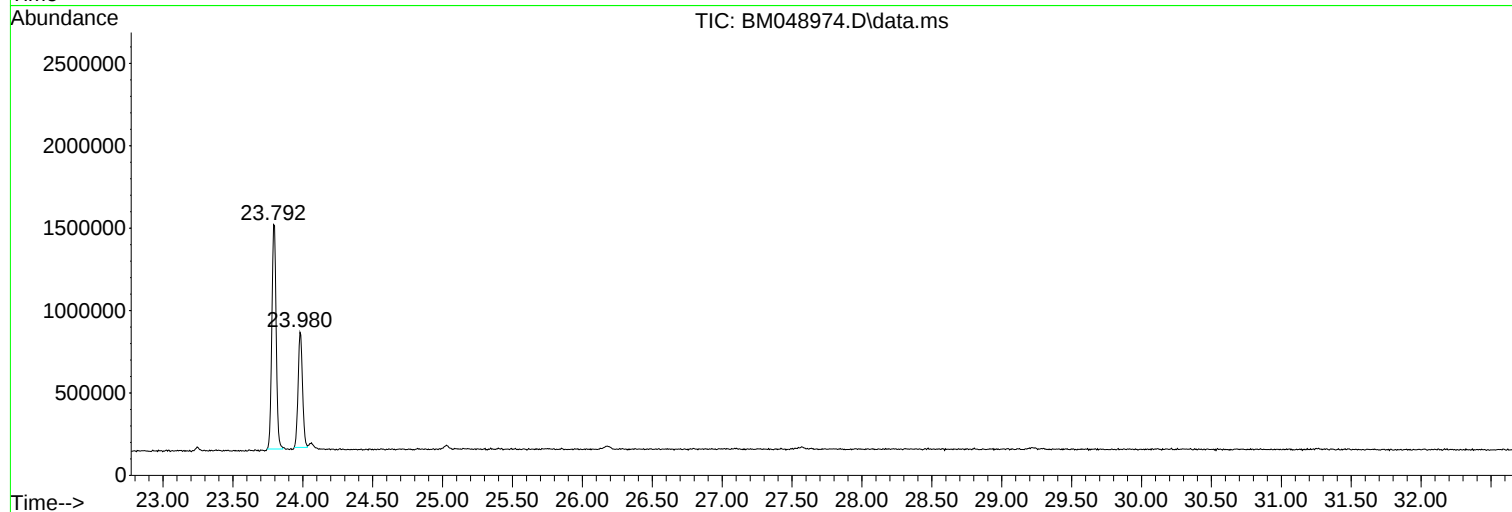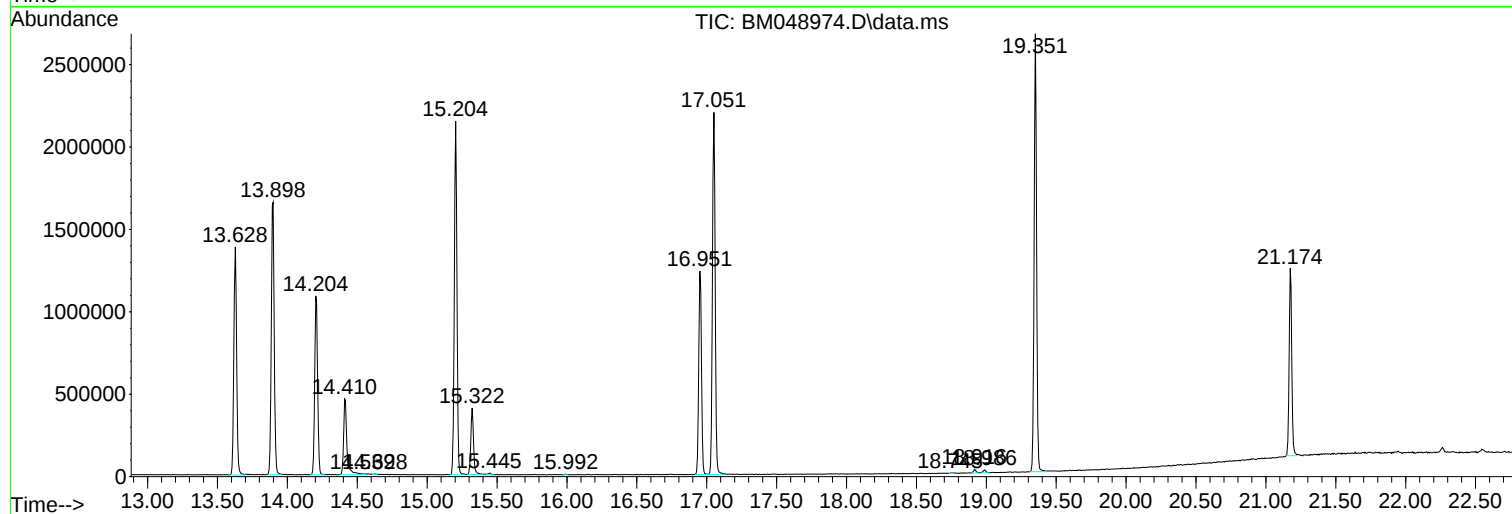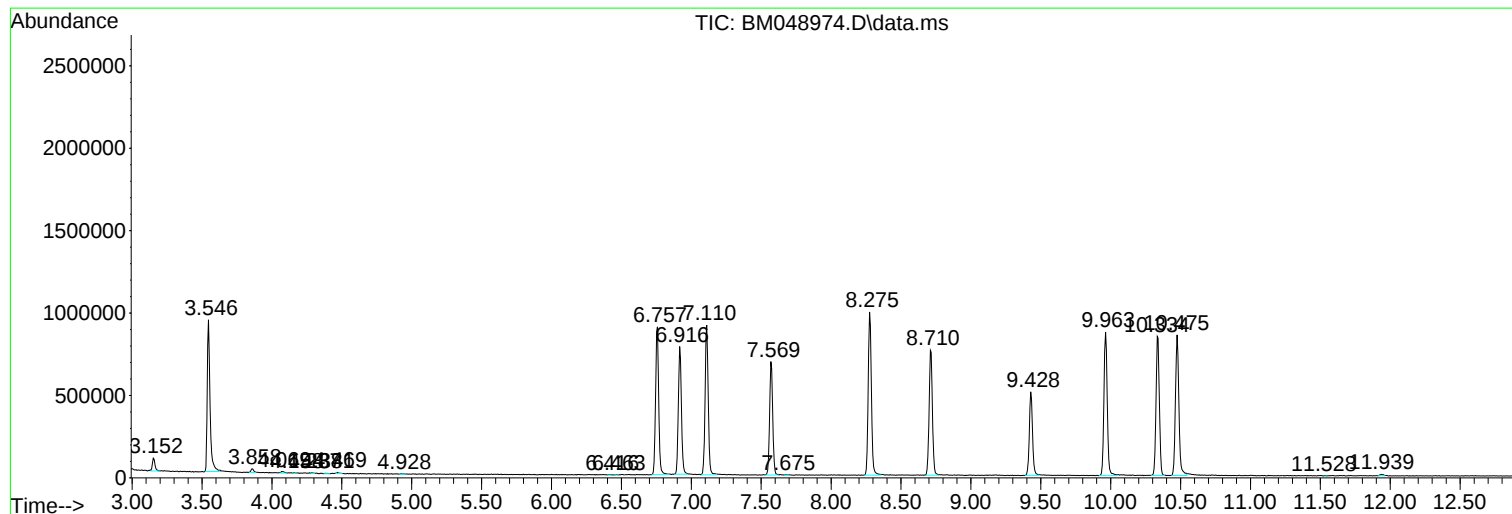

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048974.D
Acq On : 13 Dec 2024 09:45
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048974.D
Acq On : 13 Dec 2024 09:45
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------