

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048980.D
 Acq On : 13 Dec 2024 13:47
 Operator : RC/JU
 Sample : P5228-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2AT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	25	28	34	rVB	63410	77876	1.96%	0.195%
2	3.552	92	96	105	rBV	215342	319470	8.03%	0.799%
3	3.857	145	148	155	rVB3	18781	27070	0.68%	0.068%
4	3.946	161	163	170	rVB6	9848	12709	0.32%	0.032%
5	4.210	204	208	212	rVB6	14310	20274	0.51%	0.051%
6	4.352	229	232	235	rVB5	5210	6664	0.17%	0.017%
7	4.622	276	278	282	rBV5	4063	6142	0.15%	0.015%
8	4.751	295	300	306	rBV2	31769	44619	1.12%	0.112%
9	5.546	431	435	439	rBV	31799	45148	1.13%	0.113%
10	5.722	462	465	470	rVB5	5816	8421	0.21%	0.021%
11	6.528	600	602	605	rBV3	3499	4073	0.10%	0.010%
12	6.757	630	641	648	rBV	249065	412692	10.37%	1.033%
13	6.916	661	668	679	rVV	781349	1172190	29.46%	2.933%
14	7.110	693	701	711	rBV	818842	1231985	30.97%	3.083%
15	7.216	717	719	726	rVB7	7823	11448	0.29%	0.029%
16	7.569	773	779	787	rBV	729210	1124314	28.26%	2.813%
17	7.651	787	793	799	rBV	195693	297121	7.47%	0.743%
18	7.781	811	815	818	rBV5	2295	4100	0.10%	0.010%
19	8.022	851	856	859	rBV5	3923	4316	0.11%	0.011%
20	8.275	893	899	911	rBV	666336	1040387	26.15%	2.603%
21	8.657	959	964	967	rBV5	11670	18704	0.47%	0.047%
22	8.710	967	973	987	rVV	748628	1219500	30.65%	3.052%
23	8.822	988	992	997	rVV8	6920	12455	0.31%	0.031%
24	8.892	1001	1004	1008	rVB6	3806	5234	0.13%	0.013%
25	8.998	1017	1022	1025	rBV6	3166	4843	0.12%	0.012%
26	9.428	1086	1095	1102	rBV	504054	805274	20.24%	2.015%
27	9.492	1102	1106	1114	rVB	77573	126327	3.18%	0.316%
28	9.963	1179	1186	1195	rBV	892070	1418515	35.66%	3.550%
29	10.333	1242	1249	1260	rBV	920531	1513664	38.05%	3.788%
30	10.475	1265	1273	1297	rBV	729789	1289789	32.42%	3.227%
31	10.845	1331	1336	1342	rBV7	9448	16388	0.41%	0.041%
32	10.922	1348	1349	1354	rVB5	3159	3998	0.10%	0.010%
33	11.780	1488	1495	1497	rBV6	5115	9040	0.23%	0.023%
34	11.939	1517	1522	1525	rBV4	9365	16842	0.42%	0.042%
35	13.045	1708	1710	1713	rBV4	3692	4017	0.10%	0.010%
36	13.133	1719	1725	1727	rBV6	4847	8658	0.22%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048980.D
 Acq On : 13 Dec 2024 13:47
 Operator : RC/JU
 Sample : P5228-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2AT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

37	13.627	1802	1809	1818	rBV	1498086	2062902	51.85%	5.162%
38	13.892	1847	1854	1866	rBV	1785314	2578751	64.82%	6.453%
39	14.204	1900	1907	1917	rBV	1278765	1859182	46.73%	4.652%
40	14.304	1921	1924	1930	rVB3	14507	19041	0.48%	0.048%
41	14.416	1937	1943	1956	rBV	94597	198473	4.99%	0.497%
42	14.645	1976	1982	1988	rBV4	22214	36411	0.92%	0.091%
43	14.898	2021	2025	2029	rBV5	6960	9426	0.24%	0.024%
44	15.204	2067	2077	2089	rBV	2389006	3231358	81.22%	8.086%
45	15.321	2091	2097	2107	rBV	473852	614949	15.46%	1.539%
46	15.445	2114	2118	2122	rVB5	8276	11712	0.29%	0.029%
47	15.580	2138	2141	2148	rBV6	3471	7043	0.18%	0.018%
48	16.739	2336	2338	2343	rBV4	4376	4785	0.12%	0.012%
49	16.951	2368	2374	2384	rBV2	1472196	1968204	49.47%	4.925%
50	17.051	2385	2391	2405	rVB	2600267	3532017	88.78%	8.838%
51	17.639	2486	2491	2497	rBV2	85298	112615	2.83%	0.282%
52	17.874	2526	2531	2537	rBV6	7268	13870	0.35%	0.035%
53	18.562	2644	2648	2650	rBV4	3597	4692	0.12%	0.012%
54	18.915	2704	2708	2714	rBV5	21435	29978	0.75%	0.075%
55	18.986	2716	2720	2724	rBV4	21605	32076	0.81%	0.080%
56	19.156	2748	2749	2753	rBV4	8125	11477	0.29%	0.029%
57	19.351	2776	2782	2797	rVB	3278469	3978344	100.00%	9.955%
58	21.174	3087	3092	3104	rBV	1466986	1903694	47.85%	4.764%
59	23.797	3529	3538	3551	rBV	1645340	3472168	87.28%	8.688%
60	23.986	3562	3570	3579	rBV	852832	1925746	48.41%	4.819%




Sum of corrected areas: 39963181

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048980.D
Acq On : 13 Dec 2024 13:47
Operator : RC/JU
Sample : P5228-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AT1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

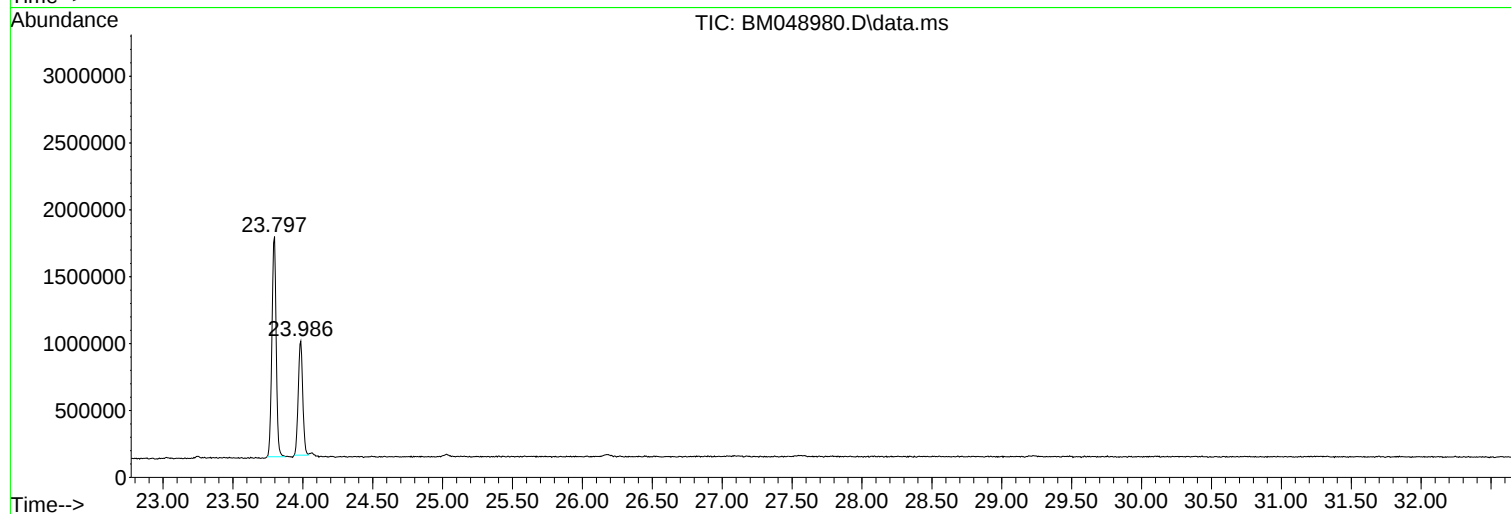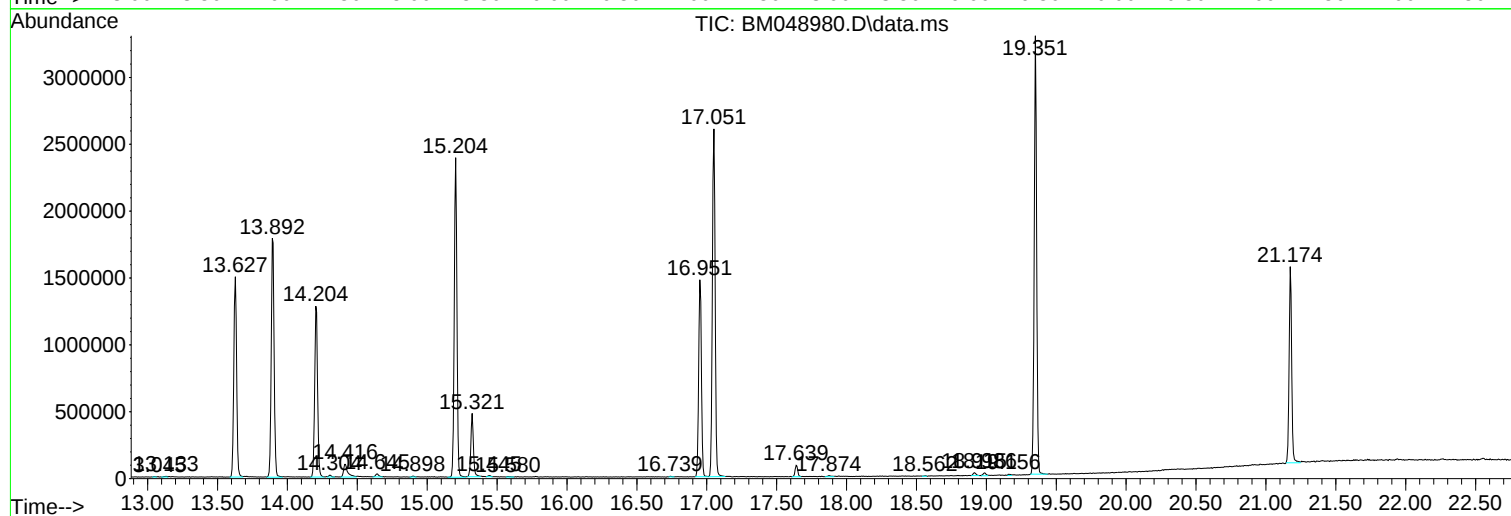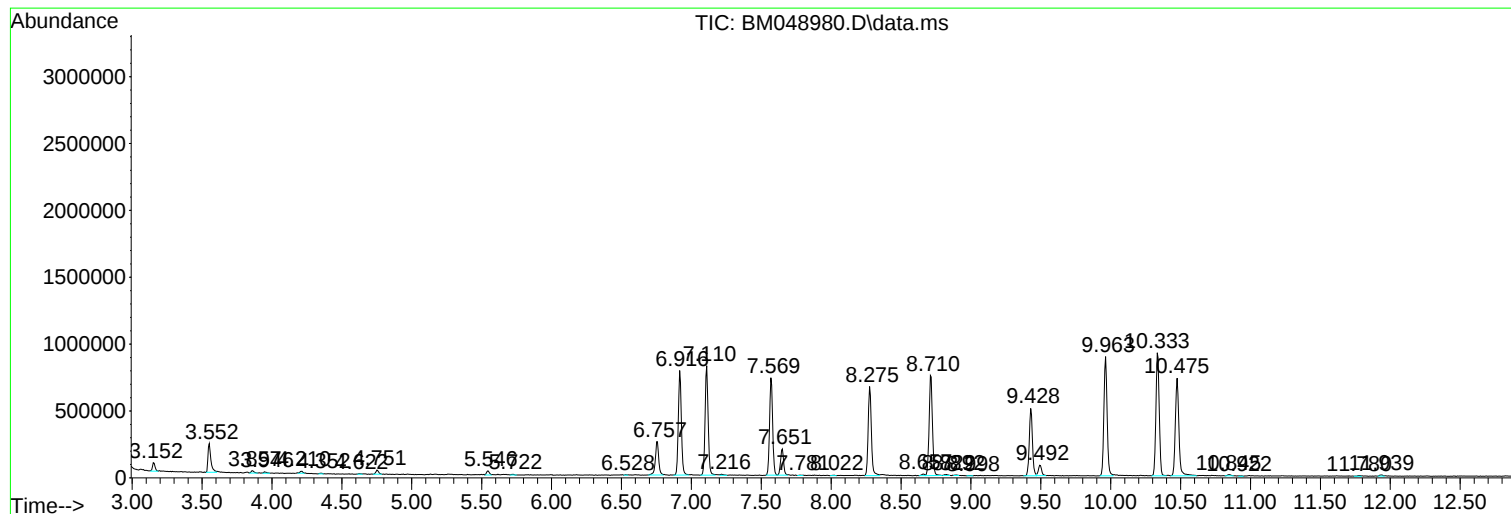

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048980.D
Acq On : 13 Dec 2024 13:47
Operator : RC/JU
Sample : P5228-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AT1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048980.D
Acq On : 13 Dec 2024 13:47
Operator : RC/JU
Sample : P5228-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AT1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc