

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048981.D
 Acq On : 13 Dec 2024 14:26
 Operator : RC/JU
 Sample : P5228-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2AT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048981.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	25	28	38	rVB	52116	72679	2.29%	0.230%
2	3.552	93	96	104	rBV	91703	142706	4.50%	0.452%
3	3.822	140	142	143	rBV2	4340	3380	0.11%	0.011%
4	3.857	145	148	153	rVB	16891	20843	0.66%	0.066%
5	3.952	161	164	167	rVB4	7093	9508	0.30%	0.030%
6	4.205	204	207	215	rVB3	21691	30229	0.95%	0.096%
7	4.346	228	231	235	rBV4	6209	8812	0.28%	0.028%
8	4.752	296	300	305	rVB2	20289	29556	0.93%	0.094%
9	5.546	430	435	443	rVB	31669	45408	1.43%	0.144%
10	5.657	453	454	460	rVV6	3841	5570	0.18%	0.018%
11	5.728	462	466	469	rBV5	5786	7995	0.25%	0.025%
12	6.269	556	558	562	rBV4	2741	3245	0.10%	0.010%
13	6.757	630	641	652	rBV	185145	327038	10.31%	1.036%
14	6.916	662	668	681	rBV	683669	1049496	33.09%	3.325%
15	7.110	694	701	711	rBV	713680	1069731	33.72%	3.389%
16	7.281	728	730	733	rVB4	4282	3494	0.11%	0.011%
17	7.569	773	779	786	rBV	608995	944271	29.77%	2.991%
18	7.651	786	793	801	rVV	197346	311218	9.81%	0.986%
19	7.793	815	817	820	rBV4	3157	3301	0.10%	0.010%
20	8.275	893	899	912	rBV	523556	820069	25.85%	2.598%
21	8.369	912	915	924	rVB7	7024	13555	0.43%	0.043%
22	8.663	960	965	967	rBV5	9625	15952	0.50%	0.051%
23	8.710	967	973	985	rVB	665948	1057367	33.33%	3.350%
24	8.816	988	991	995	rBV6	5308	6884	0.22%	0.022%
25	8.892	1000	1004	1008	rBV6	6712	9383	0.30%	0.030%
26	9.428	1088	1095	1102	rBV	435399	685400	21.61%	2.171%
27	9.492	1102	1106	1112	rVB	74492	115872	3.65%	0.367%
28	9.963	1179	1186	1198	rBV	751539	1220774	38.49%	3.867%
29	10.222	1228	1230	1233	rVB4	3968	3750	0.12%	0.012%
30	10.334	1241	1249	1258	rBV	748035	1225215	38.63%	3.881%
31	10.398	1258	1260	1263	rVB5	3831	4157	0.13%	0.013%
32	10.475	1266	1273	1286	rBV	227208	420173	13.25%	1.331%
33	10.851	1333	1337	1344	rVB5	8118	11805	0.37%	0.037%
34	10.992	1358	1361	1366	rVV5	3105	5275	0.17%	0.017%
35	11.780	1490	1495	1502	rBV8	5873	11974	0.38%	0.038%
36	11.939	1515	1522	1530	rBV3	9753	19193	0.61%	0.061%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048981.D
 Acq On : 13 Dec 2024 14:26
 Operator : RC/JU
 Sample : P5228-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2AT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

37	12.216	1568	1569	1575	rBV6	2741	3907	0.12%	0.012%
38	12.822	1670	1672	1678	rVB5	2212	3516	0.11%	0.011%
39	13.057	1709	1712	1716	rVB5	2423	3923	0.12%	0.012%
40	13.127	1718	1724	1729	rVV6	6481	12078	0.38%	0.038%
41	13.175	1729	1732	1734	rVB3	3994	4612	0.15%	0.015%
42	13.627	1802	1809	1820	rBV	1236712	1640731	51.73%	5.198%
43	13.892	1848	1854	1863	rBV	1423508	2098422	66.16%	6.647%
44	14.204	1900	1907	1919	rBV	993374	1439368	45.38%	4.560%
45	14.304	1920	1924	1928	rVB4	10356	13739	0.43%	0.044%
46	14.416	1937	1943	1958	rBV2	57573	122135	3.85%	0.387%
47	14.645	1977	1982	1990	rBV5	18137	30295	0.96%	0.096%
48	14.898	2021	2025	2030	rBV6	5222	8451	0.27%	0.027%
49	15.204	2070	2077	2085	rBV	1963059	2620507	82.62%	8.301%
50	15.321	2091	2097	2105	rBV	351285	464400	14.64%	1.471%
51	15.445	2113	2118	2122	rVB5	8259	12077	0.38%	0.038%
52	16.574	2307	2310	2312	rBV4	2928	3463	0.11%	0.011%
53	16.739	2334	2338	2340	rBV3	3852	4312	0.14%	0.014%
54	16.951	2368	2374	2384	rBV2	1131080	1477561	46.58%	4.681%
55	17.051	2384	2391	2400	rBV	2198688	2837948	89.47%	8.990%
56	17.262	2426	2427	2432	rVB4	3727	4358	0.14%	0.014%
57	17.639	2486	2491	2499	rVB	76108	97592	3.08%	0.309%
58	17.874	2527	2531	2539	rBV5	9913	16233	0.51%	0.051%
59	18.298	2600	2603	2605	rBV4	2990	3420	0.11%	0.011%
60	18.515	2638	2640	2645	rBV6	3082	4170	0.13%	0.013%
61	18.915	2704	2708	2714	rVB4	19635	27143	0.86%	0.086%
62	18.986	2716	2720	2725	rBV2	16487	22885	0.72%	0.072%
63	19.027	2725	2727	2731	rBV4	2839	3763	0.12%	0.012%
64	19.168	2747	2751	2755	rBV5	8853	11892	0.37%	0.038%
65	19.351	2776	2782	2790	rBV	2673150	3171948	100.00%	10.048%
66	21.174	3087	3092	3102	rBV	1095324	1423050	44.86%	4.508%
67	23.791	3529	3537	3548	rBV	1267377	2791361	88.00%	8.843%
68	23.980	3562	3569	3579	rBV	662392	1452833	45.80%	4.602%




Sum of corrected areas: 31567371

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048981.D
Acq On : 13 Dec 2024 14:26
Operator : RC/JU
Sample : P5228-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AT5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

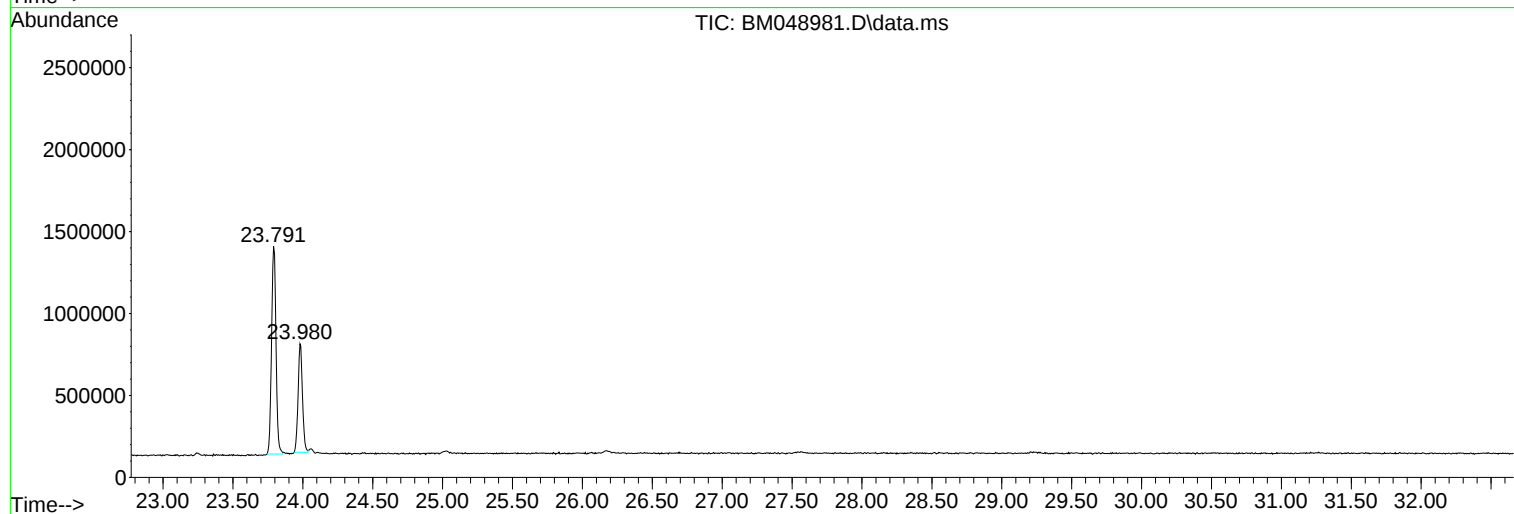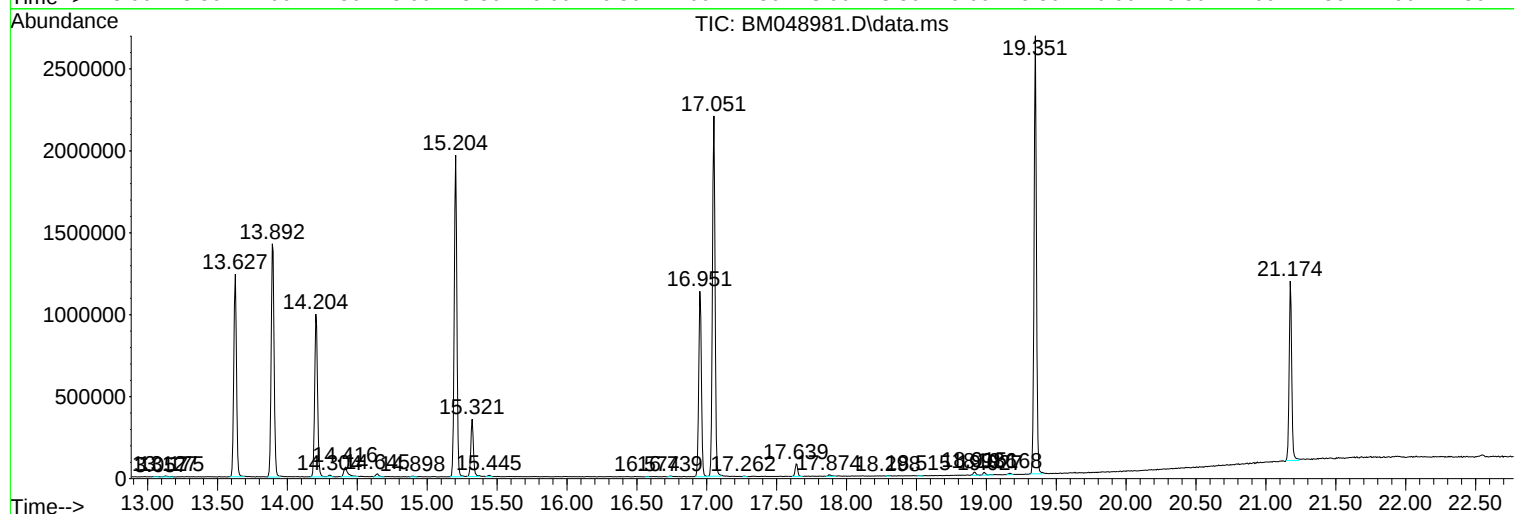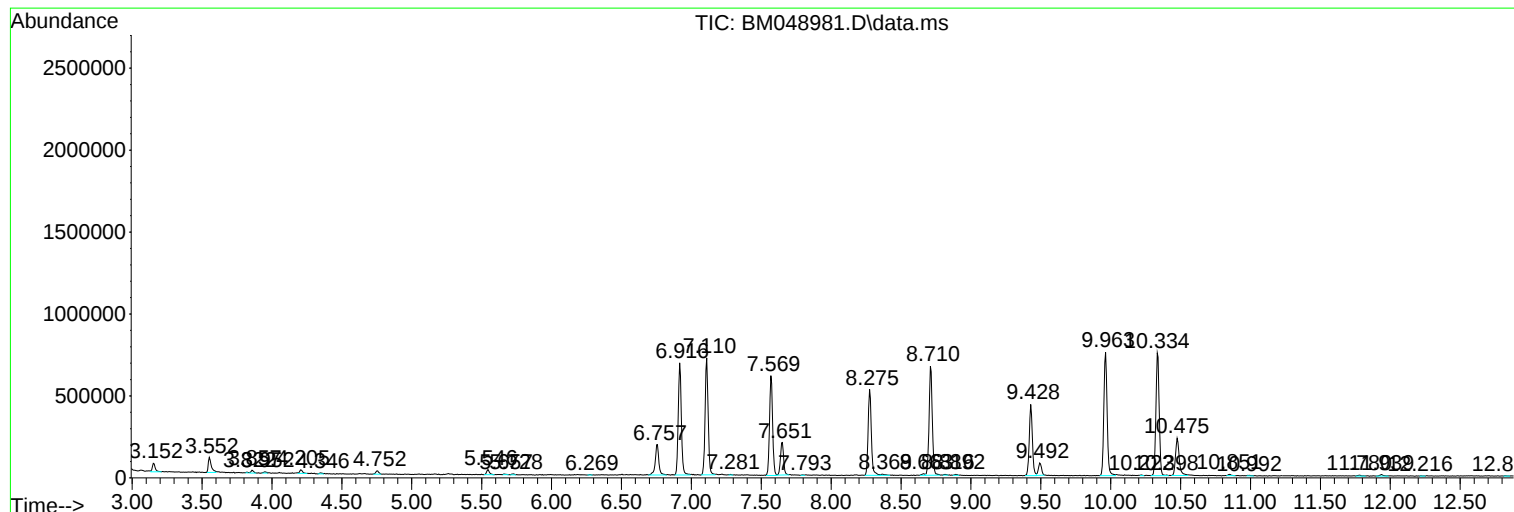

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048981.D
Acq On : 13 Dec 2024 14:26
Operator : RC/JU
Sample : P5228-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AT5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048981.D
Acq On : 13 Dec 2024 14:26
Operator : RC/JU
Sample : P5228-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AT5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc