

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048983.D
 Acq On : 13 Dec 2024 15:44
 Operator : RC/JU
 Sample : PB165613BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK613

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.151	24	28	33	rVB	55404	67303	2.71%	0.217%
2	3.546	91	95	109	rBV	744548	1080855	43.47%	3.490%
3	3.775	133	134	141	rVB5	4543	6379	0.26%	0.021%
4	3.857	144	148	152	rVB2	12523	14960	0.60%	0.048%
5	4.228	209	211	214	rVB4	3416	2832	0.11%	0.009%
6	4.357	232	233	237	rVB4	3086	3800	0.15%	0.012%
7	4.393	237	239	241	rBV3	2571	3122	0.13%	0.010%
8	4.634	276	280	281	rBV4	2726	3486	0.14%	0.011%
9	4.875	320	321	324	rBV3	3512	3130	0.13%	0.010%
10	5.028	343	347	348	rBV4	2279	3010	0.12%	0.010%
11	5.557	436	437	444	rBV5	2797	4801	0.19%	0.016%
12	5.745	466	469	470	rVB2	4582	3700	0.15%	0.012%
13	5.763	470	472	474	rBV2	2655	3262	0.13%	0.011%
14	6.528	601	602	606	rBV4	2476	2519	0.10%	0.008%
15	6.581	607	611	614	rVB6	2642	3825	0.15%	0.012%
16	6.698	628	631	634	rBV4	2569	3045	0.12%	0.010%
17	6.757	634	641	654	rBV	685311	1080069	43.44%	3.487%
18	6.916	662	668	679	rVB	558014	860491	34.61%	2.778%
19	7.110	694	701	716	rBV	663265	1040937	41.87%	3.361%
20	7.569	772	779	789	rBV	632798	983263	39.55%	3.175%
21	8.057	859	862	865	rBV4	2844	3655	0.15%	0.012%
22	8.275	890	899	908	rBV	757880	1192881	47.98%	3.852%
23	8.710	967	973	986	rBV	552659	878790	35.35%	2.838%
24	9.022	1025	1026	1030	rBV4	2749	3789	0.15%	0.012%
25	9.428	1088	1095	1106	rBV	346139	552607	22.23%	1.784%
26	9.786	1152	1156	1159	rBV3	2964	2786	0.11%	0.009%
27	9.833	1161	1164	1167	rVB4	2535	3238	0.13%	0.010%
28	9.857	1167	1168	1171	rBV3	3166	2739	0.11%	0.009%
29	9.963	1179	1186	1200	rBV	644532	1062725	42.74%	3.431%
30	10.333	1242	1249	1259	rVB	783372	1259690	50.67%	4.067%
31	10.475	1264	1273	1287	rBV	598370	1091910	43.92%	3.526%
32	10.663	1303	1305	1309	rVB3	3323	2915	0.12%	0.009%
33	10.775	1322	1324	1327	rVB4	2804	2717	0.11%	0.009%
34	11.016	1363	1365	1367	rBV3	3127	3182	0.13%	0.010%
35	11.269	1406	1408	1411	rBV3	2903	3078	0.12%	0.010%
36	11.598	1462	1464	1470	rVB5	2155	3354	0.13%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048983.D
 Acq On : 13 Dec 2024 15:44
 Operator : RC/JU
 Sample : PB165613BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK613

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

37	11.939	1516	1522	1528	rBV7	7052	15326	0.62%	0.049%
38	12.557	1624	1627	1631	rVV5	1830	3136	0.13%	0.010%
39	12.986	1697	1700	1703	rBV5	1996	2538	0.10%	0.008%
40	13.074	1712	1715	1716	rBV2	2512	2904	0.12%	0.009%
41	13.186	1733	1734	1737	rVB2	2994	2511	0.10%	0.008%
42	13.363	1760	1764	1767	rVB6	1901	2764	0.11%	0.009%
43	13.545	1791	1795	1797	rBV4	2066	2604	0.10%	0.008%
44	13.627	1803	1809	1818	rBV	988242	1403159	56.44%	4.531%
45	13.804	1837	1839	1845	rBV7	2155	3948	0.16%	0.013%
46	13.892	1847	1854	1866	rBV	1216317	1770802	71.22%	5.718%
47	13.986	1869	1870	1876	rVV3	2894	2999	0.12%	0.010%
48	14.039	1876	1879	1882	rVB4	1977	2527	0.10%	0.008%
49	14.074	1882	1885	1888	rBV5	2225	2621	0.11%	0.008%
50	14.204	1901	1907	1916	rBV	1045938	1472147	59.21%	4.753%
51	14.410	1936	1942	1956	rBV	311830	548254	22.05%	1.770%
52	15.039	2047	2049	2053	rBV4	1980	2918	0.12%	0.009%
53	15.204	2070	2077	2086	rVV	1515587	2099070	84.43%	6.778%
54	15.321	2091	2097	2108	rBV	268281	371551	14.94%	1.200%
55	15.445	2115	2118	2119	rBV2	6293	5275	0.21%	0.017%
56	15.521	2129	2131	2136	rBV5	1627	2617	0.11%	0.008%
57	15.662	2153	2155	2158	rVB4	2230	2697	0.11%	0.009%
58	16.133	2231	2235	2237	rBV2	3126	4316	0.17%	0.014%
59	16.604	2311	2315	2316	rBV4	2709	3101	0.12%	0.010%
60	16.745	2334	2339	2344	rVB6	3674	5450	0.22%	0.018%
61	16.951	2368	2374	2381	rBV	1224956	1632274	65.65%	5.271%
62	17.051	2384	2391	2401	rVV	1658811	2205735	88.72%	7.122%
63	17.574	2475	2480	2482	rBV5	2084	2771	0.11%	0.009%
64	17.645	2487	2492	2493	rVB4	3233	3215	0.13%	0.010%
65	18.368	2613	2615	2618	rBV3	2353	2882	0.12%	0.009%
66	18.498	2636	2637	2639	rBV2	2862	2519	0.10%	0.008%
67	18.762	2680	2682	2685	rBV4	2873	4181	0.17%	0.014%
68	18.868	2698	2700	2701	rBV2	3753	2789	0.11%	0.009%
69	18.915	2704	2708	2713	rVV4	16277	23770	0.96%	0.077%
70	18.986	2716	2720	2725	rVB3	12301	18446	0.74%	0.060%
71	19.115	2741	2742	2744	rBV2	4003	3496	0.14%	0.011%
72	19.174	2750	2752	2755	rVB4	4383	3175	0.13%	0.010%
73	19.350	2776	2782	2793	rBV	1917060	2486250	100.00%	8.028%
74	21.174	3087	3092	3100	rBV	1199703	1650492	66.38%	5.329%
75	23.791	3529	3537	3548	rBV	1066868	2275783	91.53%	7.348%
76	23.985	3562	3570	3580	rBV	749693	1671959	67.25%	5.399%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048983.D
Acq On : 13 Dec 2024 15:44
Operator : RC/JU
Sample : PB165613BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK613

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 30969817

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048983.D
Acq On : 13 Dec 2024 15:44
Operator : RC/JU
Sample : PB165613BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK613

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

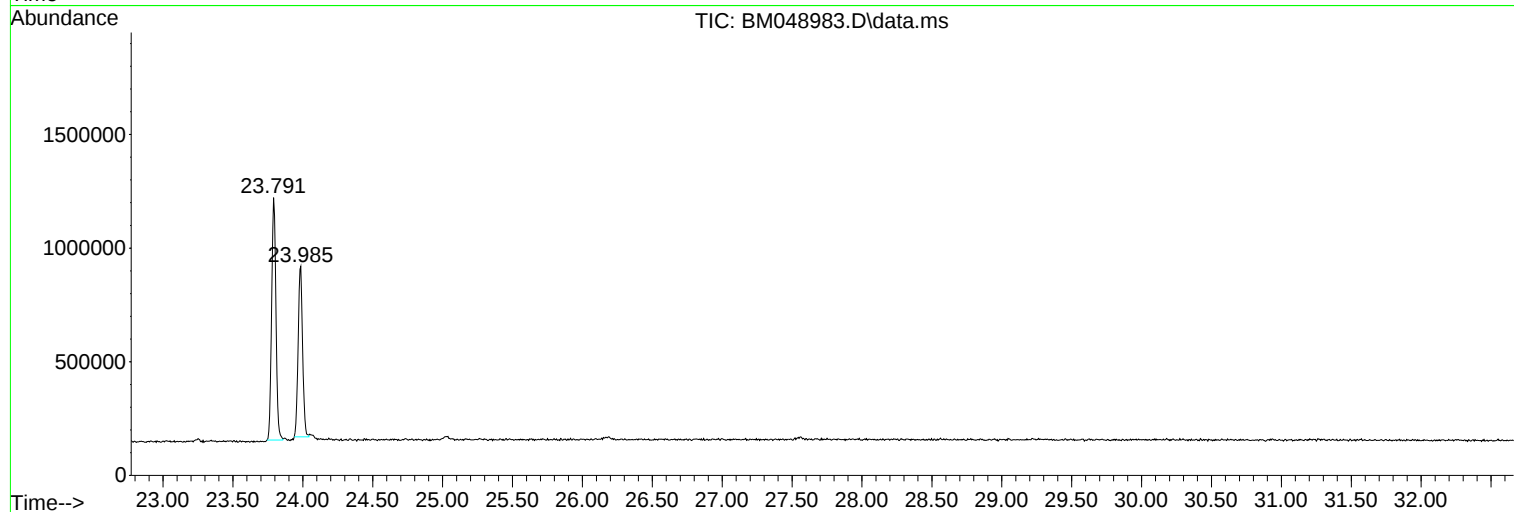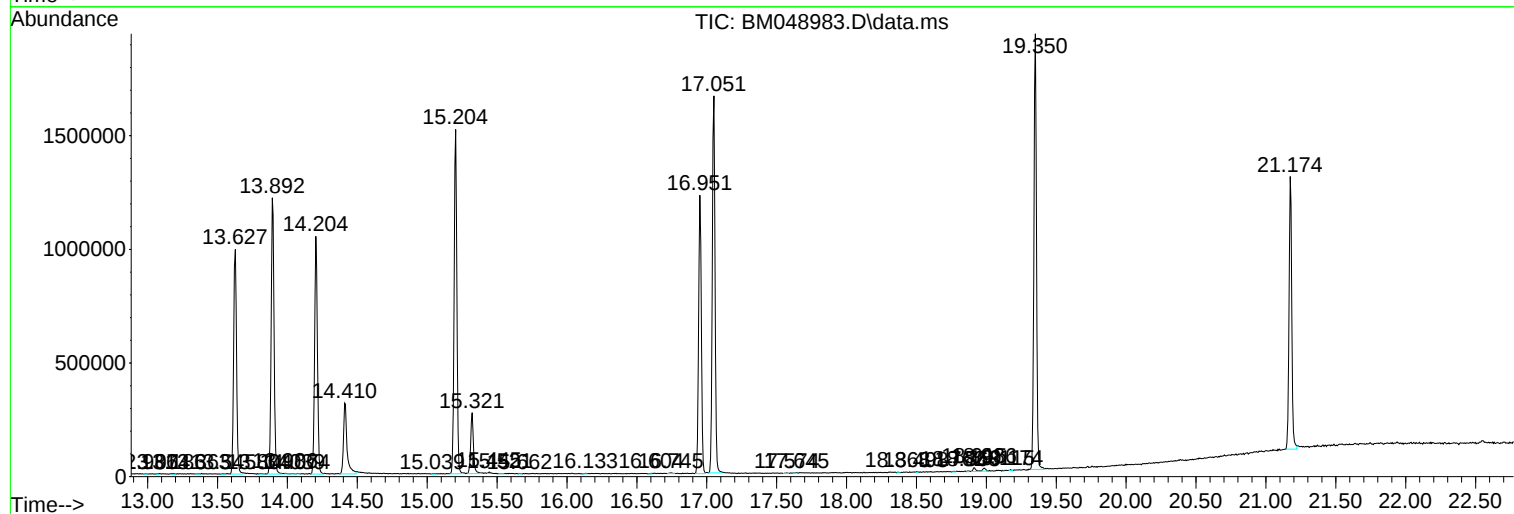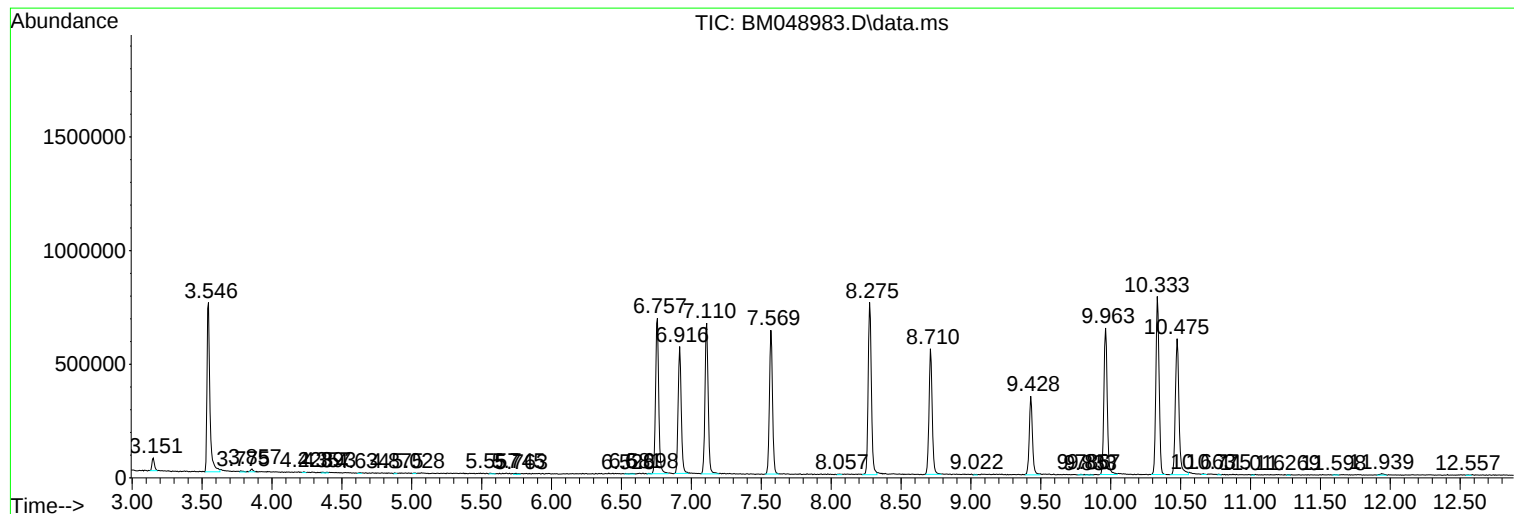

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048983.D
Acq On : 13 Dec 2024 15:44
Operator : RC/JU
Sample : PB165613BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK613

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048983.D
Acq On : 13 Dec 2024 15:44
Operator : RC/JU
Sample : PB165613BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK613

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc