

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048984.D
 Acq On : 13 Dec 2024 16:23
 Operator : RC/JU
 Sample : PB165610BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK610

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	24	28	35	rVB	49457	65652	2.92%	0.240%
2	3.316	54	56	57	rBV	3729	2257	0.10%	0.008%
3	3.540	90	94	118	rBV	652512	969534	43.15%	3.545%
4	3.857	144	148	153	rBV2	13224	17750	0.79%	0.065%
5	4.187	202	204	207	rBV3	2731	2856	0.13%	0.010%
6	5.928	496	500	506	rBV8	1801	4106	0.18%	0.015%
7	6.163	538	540	545	rVB5	2138	2707	0.12%	0.010%
8	6.216	545	549	550	rBV4	2487	2652	0.12%	0.010%
9	6.304	561	564	565	rBV2	3336	3046	0.14%	0.011%
10	6.351	569	572	575	rBV4	1896	2697	0.12%	0.010%
11	6.422	582	584	585	rBV2	2456	2251	0.10%	0.008%
12	6.493	593	596	599	rBV4	2797	2567	0.11%	0.009%
13	6.751	634	640	654	rBV	598489	939566	41.81%	3.435%
14	6.916	661	668	678	rBV	504958	771301	34.32%	2.820%
15	7.110	693	701	712	rVV	602649	918473	40.87%	3.358%
16	7.193	712	715	717	rVV4	3294	4626	0.21%	0.017%
17	7.216	717	719	720	rVB2	3353	2335	0.10%	0.009%
18	7.569	773	779	788	rBV	546615	831221	36.99%	3.039%
19	7.869	827	830	831	rVB3	2723	2689	0.12%	0.010%
20	7.910	835	837	839	rBV3	2384	2571	0.11%	0.009%
21	8.210	884	888	890	rBV3	2040	2260	0.10%	0.008%
22	8.275	892	899	910	rBV	682023	1053649	46.89%	3.852%
23	8.569	946	949	952	rBV2	1769	2274	0.10%	0.008%
24	8.710	966	973	986	rBV	468815	777300	34.59%	2.842%
25	8.822	990	992	995	rVB3	1972	2536	0.11%	0.009%
26	8.857	995	998	1001	rBV5	2790	2993	0.13%	0.011%
27	8.951	1012	1014	1017	rBV2	2225	2340	0.10%	0.009%
28	9.075	1031	1035	1038	rBV6	2558	3859	0.17%	0.014%
29	9.192	1051	1055	1059	rVB5	2200	2900	0.13%	0.011%
30	9.345	1078	1081	1084	rBV5	2249	2935	0.13%	0.011%
31	9.369	1084	1085	1088	rVB3	2561	2411	0.11%	0.009%
32	9.428	1088	1095	1106	rBV	289863	478448	21.29%	1.749%
33	9.645	1129	1132	1134	rVB4	2284	2289	0.10%	0.008%
34	9.763	1151	1152	1155	rBV3	2009	2292	0.10%	0.008%
35	9.963	1179	1186	1202	rVV	574785	931488	41.45%	3.406%
36	10.334	1241	1249	1257	rVB	668994	1076295	47.90%	3.935%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048984.D
 Acq On : 13 Dec 2024 16:23
 Operator : RC/JU
 Sample : PB165610BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK610

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

37	10.475	1266	1273	1289	rBV	534847	958284	42.64%	3.504%
38	10.845	1332	1336	1339	rVB5	2332	3507	0.16%	0.013%
39	10.875	1339	1341	1344	rBV3	2860	2878	0.13%	0.011%
40	10.992	1358	1361	1363	rBV3	2071	2257	0.10%	0.008%
41	11.416	1429	1433	1437	rVB5	1402	2411	0.11%	0.009%
42	11.939	1518	1522	1524	rBV2	5278	6161	0.27%	0.023%
43	11.963	1524	1526	1530	rVV4	2505	2597	0.12%	0.009%
44	12.004	1532	1533	1536	rBV3	2926	2593	0.12%	0.009%
45	12.092	1546	1548	1553	rVB6	2391	3327	0.15%	0.012%
46	12.280	1575	1580	1581	rBV3	2438	3088	0.14%	0.011%
47	13.298	1750	1753	1756	rBV3	1724	2341	0.10%	0.009%
48	13.333	1758	1759	1764	rVB4	2422	3035	0.14%	0.011%
49	13.627	1803	1809	1819	rBV	884446	1212723	53.97%	4.434%
50	13.745	1827	1829	1832	rVB2	2903	2311	0.10%	0.008%
51	13.892	1848	1854	1864	rVV	1058860	1548327	68.90%	5.661%
52	14.204	1899	1907	1916	rVV	908144	1278874	56.91%	4.676%
53	14.410	1936	1942	1956	rBV	275904	473433	21.07%	1.731%
54	14.498	1956	1957	1964	rVV7	7969	14741	0.66%	0.054%
55	14.569	1968	1969	1976	rVB6	2801	4325	0.19%	0.016%
56	15.204	2070	2077	2091	rBV	1362284	1890325	84.12%	6.911%
57	15.321	2091	2097	2106	rVV	224235	307091	13.67%	1.123%
58	15.445	2114	2118	2122	rVB6	4996	7976	0.35%	0.029%
59	15.586	2141	2142	2149	rVB6	1574	3045	0.14%	0.011%
60	15.998	2210	2212	2215	rVV5	2215	2722	0.12%	0.010%
61	16.045	2217	2220	2222	rBV4	1903	2442	0.11%	0.009%
62	16.251	2251	2255	2256	rVB3	2056	2464	0.11%	0.009%
63	16.733	2333	2337	2339	rBV3	3078	4720	0.21%	0.017%
64	16.951	2367	2374	2380	rBV2	1074911	1418112	63.11%	5.185%
65	17.051	2384	2391	2404	rVV	1502397	2002449	89.11%	7.321%
66	17.262	2424	2427	2429	rBV3	1753	2290	0.10%	0.008%
67	17.333	2438	2439	2442	rBV2	3858	3194	0.14%	0.012%
68	17.433	2453	2456	2460	rBV5	3408	4003	0.18%	0.015%
69	17.880	2528	2532	2535	rBV4	2924	4777	0.21%	0.017%
70	17.915	2535	2538	2541	rBV4	2080	3415	0.15%	0.012%
71	18.592	2650	2653	2654	rBV3	3745	2384	0.11%	0.009%
72	18.915	2704	2708	2713	rVB4	12532	19115	0.85%	0.070%
73	18.980	2716	2719	2727	rVB4	9652	16828	0.75%	0.062%
74	19.351	2776	2782	2794	rBV	1767451	2247138	100.00%	8.216%
75	19.433	2794	2796	2798	rVB3	3819	3045	0.14%	0.011%
76	19.762	2850	2852	2856	rBV5	4589	4571	0.20%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048984.D
Acq On : 13 Dec 2024 16:23
Operator : RC/JU
Sample : PB165610BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK610

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Title : SVOA CALIBRATION

77	21.174	3087	3092	3103	rBV	1051173	1405963	62.57%	5.140%
78	23.786	3529	3536	3550	rBV	948277	2052867	91.35%	7.506%
79	23.980	3561	3569	3579	rBV	666435	1515583	67.45%	5.541%




Sum of corrected areas: 27350858

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048984.D
Acq On : 13 Dec 2024 16:23
Operator : RC/JU
Sample : PB165610BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK610

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

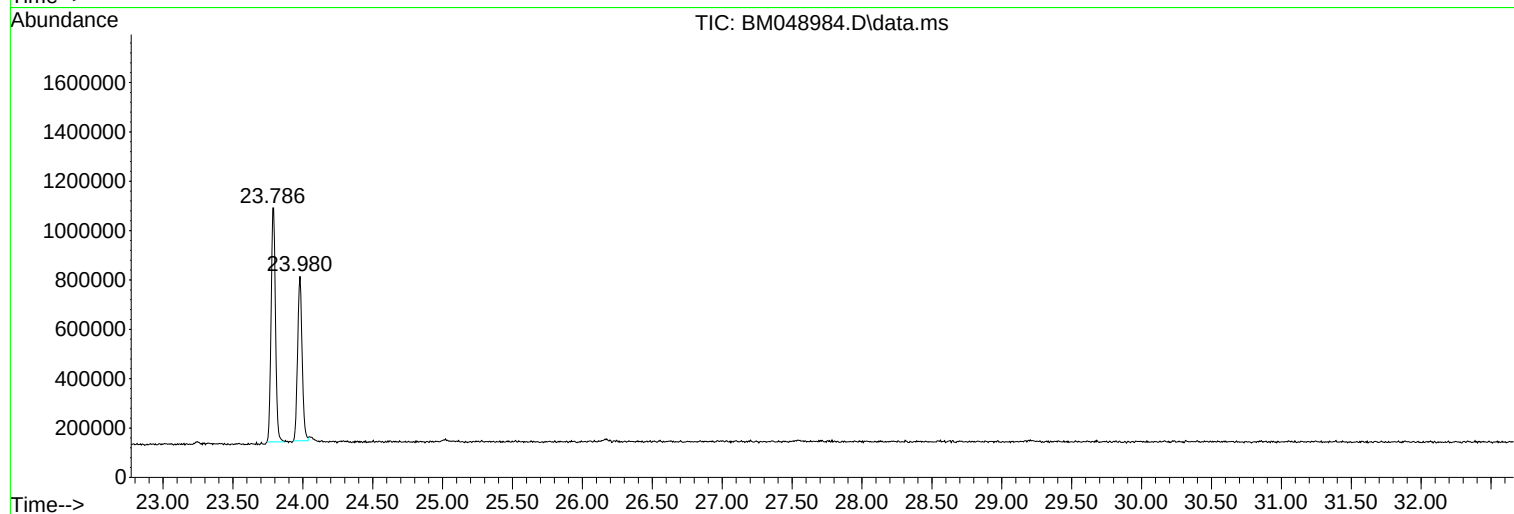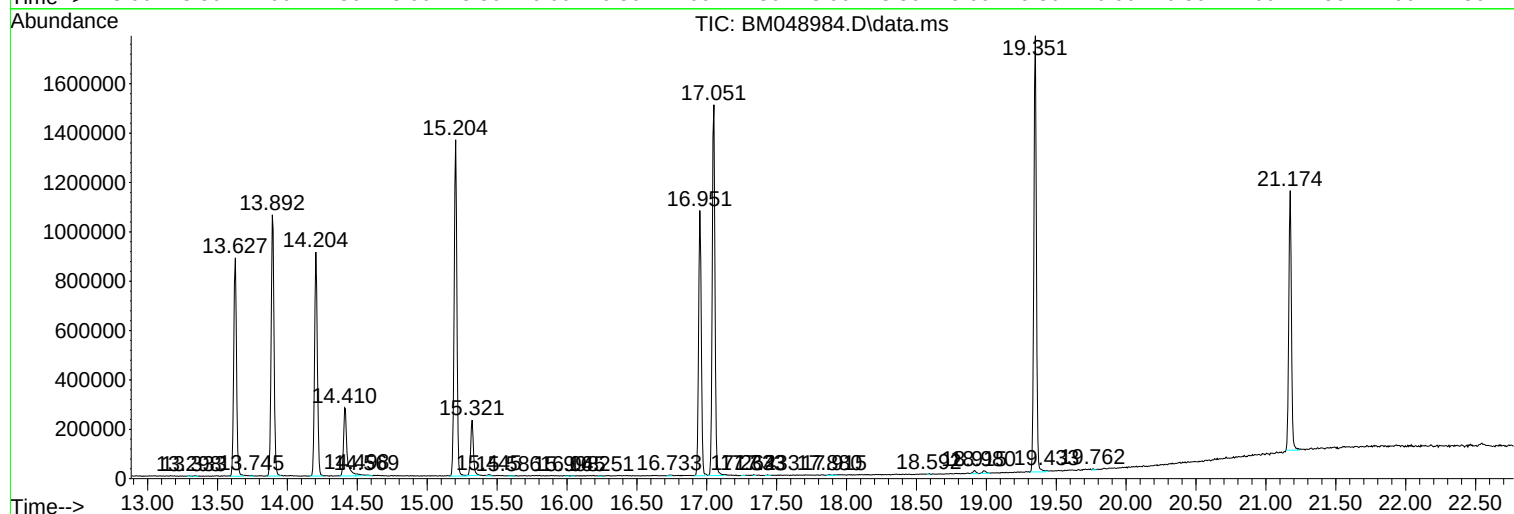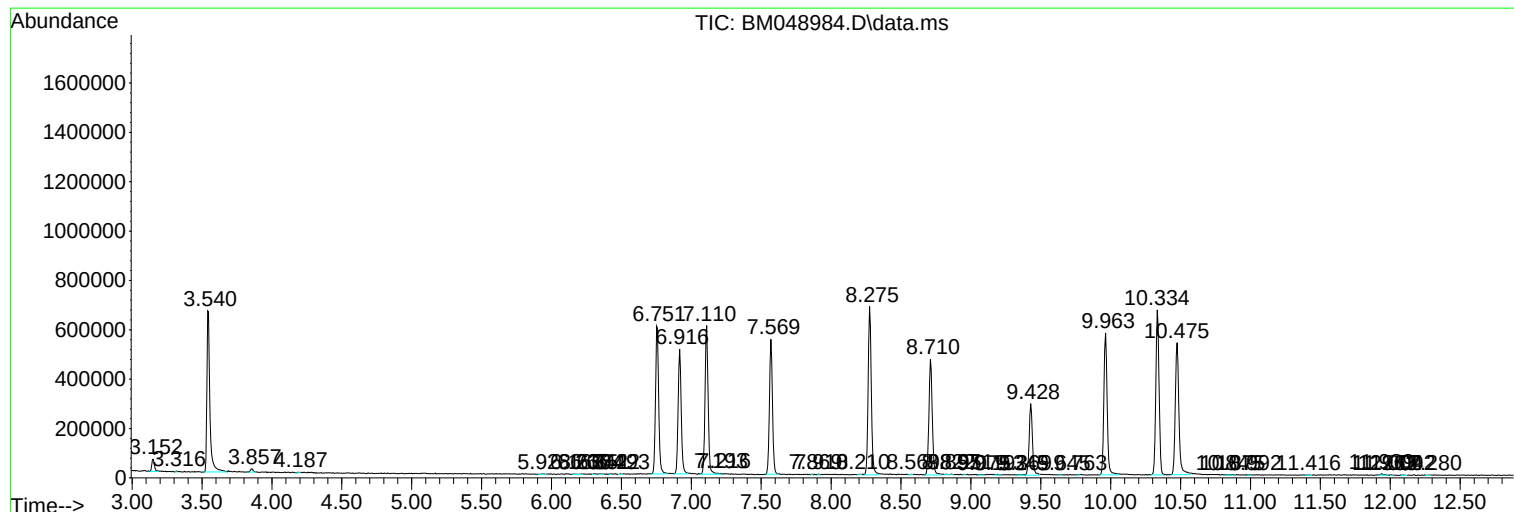

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048984.D
Acq On : 13 Dec 2024 16:23
Operator : RC/JU
Sample : PB165610BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK610

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048984.D
Acq On : 13 Dec 2024 16:23
Operator : RC/JU
Sample : PB165610BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK610

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc