

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048985.D
 Acq On : 13 Dec 2024 17:02
 Operator : RC/JU
 Sample : P5228-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E29R6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048985.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	25	28	35	rVB	47142	61472	1.94%	0.200%
2	3.546	92	95	106	rBV	171751	272724	8.59%	0.885%
3	3.858	145	148	155	rVB4	14106	18879	0.59%	0.061%
4	4.028	175	177	179	rBV3	3314	3242	0.10%	0.011%
5	4.364	229	234	246	rVB	585748	833583	26.25%	2.706%
6	4.752	296	300	306	rVV	33093	46252	1.46%	0.150%
7	6.752	634	640	649	rVV	173960	281381	8.86%	0.913%
8	6.916	662	668	682	rVB	611877	924508	29.11%	3.001%
9	7.110	694	701	713	rBV	608940	945480	29.77%	3.069%
10	7.210	716	718	724	rVB7	5920	8284	0.26%	0.027%
11	7.316	733	736	741	rBV6	3014	4827	0.15%	0.016%
12	7.410	746	752	755	rBV6	3344	6632	0.21%	0.022%
13	7.569	771	779	789	rBV	541370	858649	27.03%	2.787%
14	8.163	875	880	881	rBV4	1971	3302	0.10%	0.011%
15	8.275	890	899	914	rBV	478241	751372	23.66%	2.439%
16	8.710	966	973	985	rBV	585766	947838	29.84%	3.077%
17	8.851	992	997	999	rBV6	3267	6207	0.20%	0.020%
18	9.428	1087	1095	1103	rBV	382401	592254	18.65%	1.922%
19	9.557	1113	1117	1118	rVB4	2668	3210	0.10%	0.010%
20	9.963	1179	1186	1196	rBV	665920	1072557	33.77%	3.481%
21	10.334	1242	1249	1263	rVB	702527	1124569	35.41%	3.650%
22	10.475	1264	1273	1288	rBV	558090	990805	31.20%	3.216%
23	11.163	1387	1390	1397	rBV7	3790	8128	0.26%	0.026%
24	11.716	1481	1484	1488	rVB4	2310	3179	0.10%	0.010%
25	11.934	1515	1521	1527	rBV5	5741	11438	0.36%	0.037%
26	12.992	1697	1701	1703	rBV3	2564	3546	0.11%	0.012%
27	13.051	1708	1711	1716	rVB5	2098	4040	0.13%	0.013%
28	13.134	1723	1725	1729	rVB5	3201	3298	0.10%	0.011%
29	13.628	1802	1809	1820	rBV	1105752	1507347	47.46%	4.893%
30	13.892	1846	1854	1861	rBV	1311386	1898478	59.77%	6.162%
31	14.204	1900	1907	1918	rBV	946569	1337104	42.10%	4.340%
32	14.416	1934	1943	1958	rBV	59698	133570	4.21%	0.434%
33	15.204	2070	2077	2091	rBV	1943640	2475919	77.96%	8.036%
34	15.322	2091	2097	2106	rBV	340703	458605	14.44%	1.489%
35	15.439	2113	2117	2123	rVB6	6731	12130	0.38%	0.039%
36	15.580	2135	2141	2146	rBV	35987	54241	1.71%	0.176%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048985.D
 Acq On : 13 Dec 2024 17:02
 Operator : RC/JU
 Sample : P5228-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E29R6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

37	16.463	2289	2291	2294	rBV3	2963	3269	0.10%	0.011%
38	16.551	2303	2306	2308	rBV3	2849	4258	0.13%	0.014%
39	16.739	2335	2338	2343	rVB4	2757	3710	0.12%	0.012%
40	16.951	2368	2374	2384	rBV	1084421	1418857	44.67%	4.605%
41	17.051	2384	2391	2405	rVV	2047229	2779893	87.53%	9.023%
42	17.745	2503	2509	2511	rBV5	2638	3378	0.11%	0.011%
43	17.874	2526	2531	2538	rBV5	26427	43459	1.37%	0.141%
44	18.169	2576	2581	2582	rBV4	3217	3639	0.11%	0.012%
45	18.439	2625	2627	2631	rBV5	3113	3331	0.10%	0.011%
46	18.716	2672	2674	2676	rBV3	3239	3408	0.11%	0.011%
47	18.916	2704	2708	2712	rBV4	18030	26228	0.83%	0.085%
48	18.986	2716	2720	2723	rVV3	15783	19686	0.62%	0.064%
49	19.163	2747	2750	2759	rBV10	12020	21754	0.68%	0.071%
50	19.351	2776	2782	2792	rBV	2543127	3176070	100.00%	10.309%
51	21.174	3087	3092	3102	rBV	1066780	1389480	43.75%	4.510%
52	23.792	3529	3537	3548	rBV	1326260	2792860	87.93%	9.065%
53	23.980	3561	3569	3577	rBV	651551	1446383	45.54%	4.695%




Sum of corrected areas: 30808713

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048985.D
Acq On : 13 Dec 2024 17:02
Operator : RC/JU
Sample : P5228-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29R6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

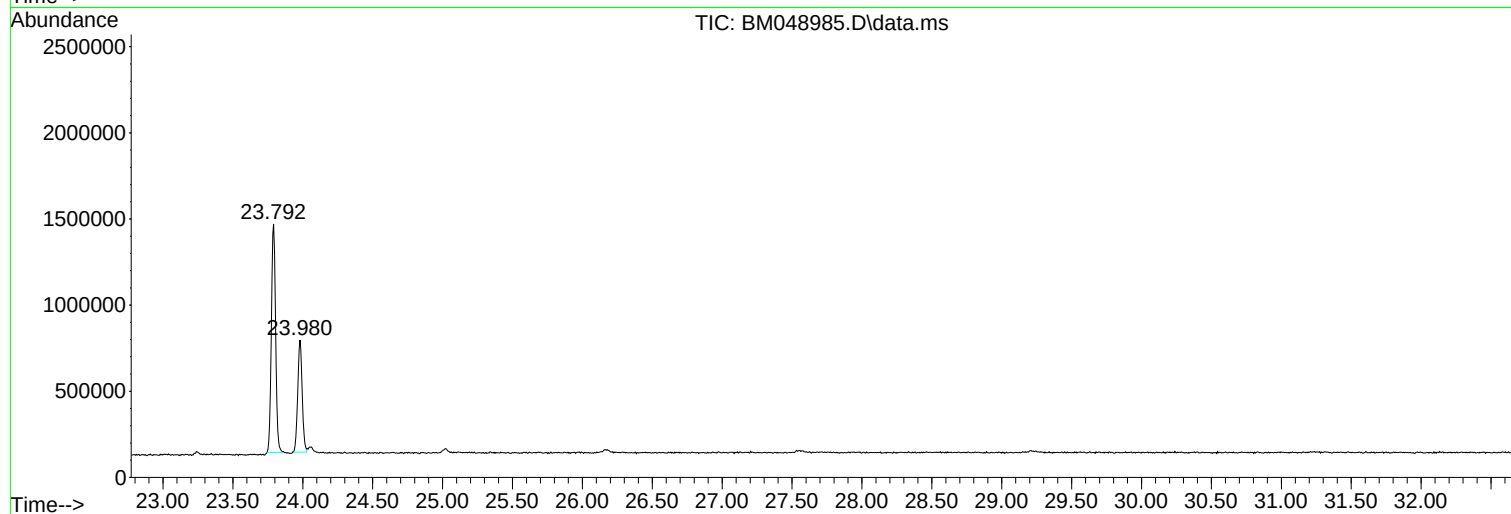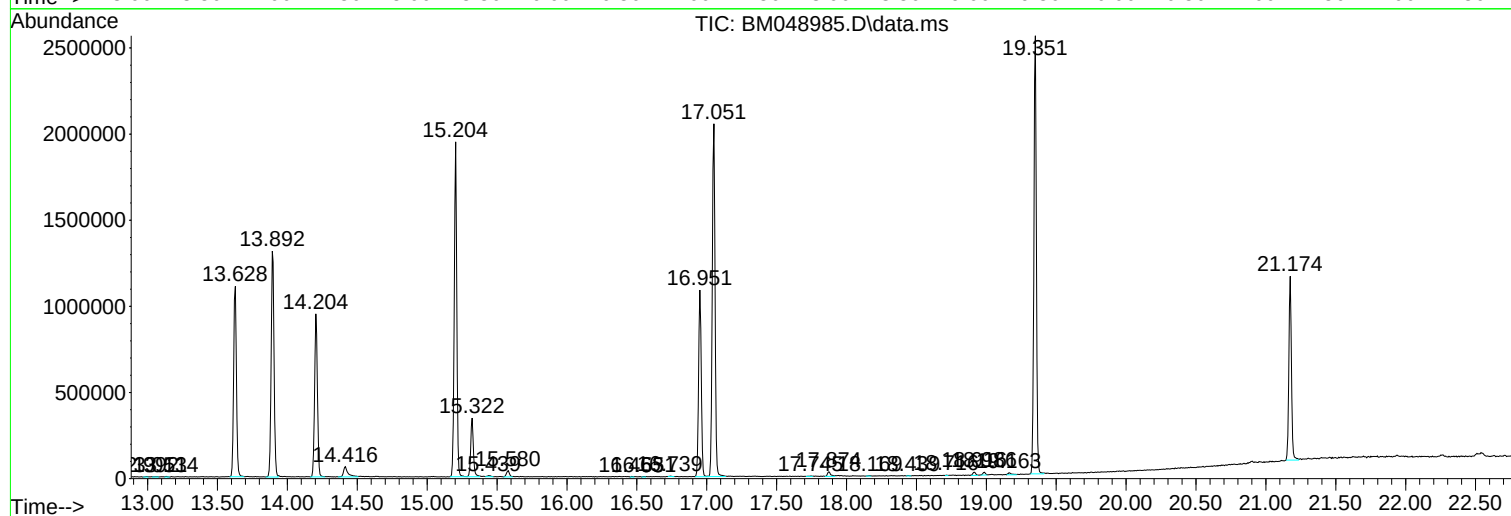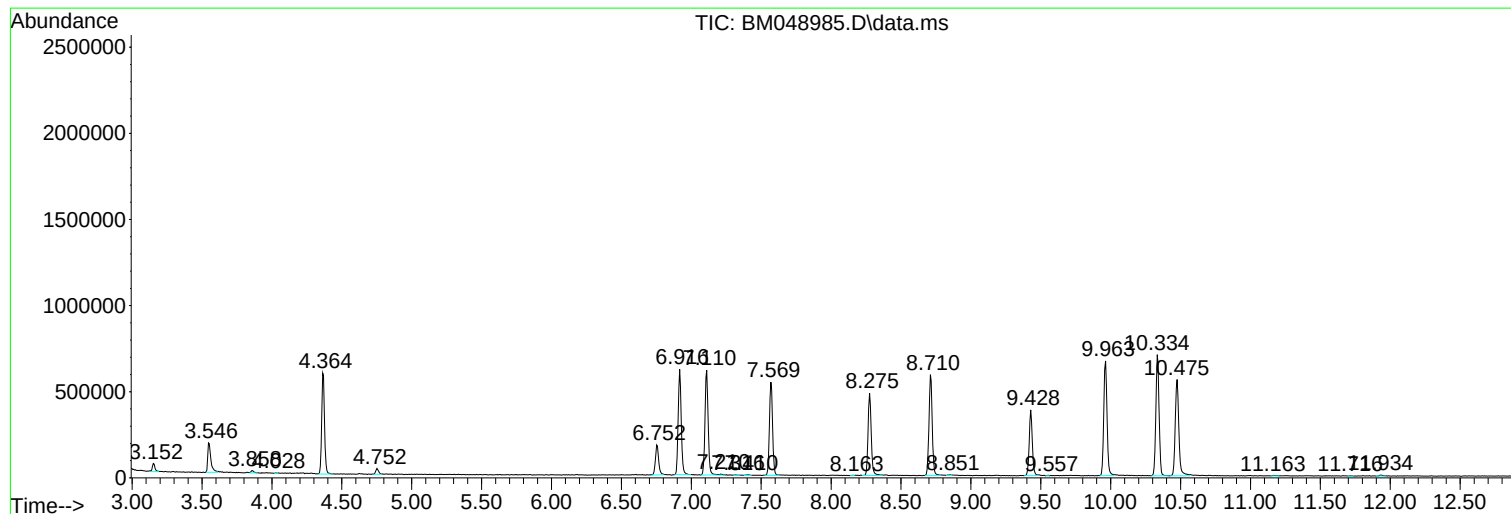

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048985.D
Acq On : 13 Dec 2024 17:02
Operator : RC/JU
Sample : P5228-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29R6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048985.D
Acq On : 13 Dec 2024 17:02
Operator : RC/JU
Sample : P5228-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29R6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------