

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048990.D
 Acq On : 13 Dec 2024 20:16
 Operator : RC/JU
 Sample : P5247-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7T2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	25	28	32	rBV	46188	49772	1.48%	0.149%
2	3.552	91	96	111	rBV	203290	351272	10.46%	1.054%
3	3.858	144	148	154	rVB	54510	70414	2.10%	0.211%
4	3.952	162	164	166	rBV3	4125	3423	0.10%	0.010%
5	4.216	206	209	212	rVB3	6970	7774	0.23%	0.023%
6	4.622	276	278	283	rVB4	3120	4422	0.13%	0.013%
7	4.752	295	300	304	rBV3	12427	21625	0.64%	0.065%
8	6.751	634	640	652	rVB	210461	338931	10.09%	1.017%
9	6.916	662	668	678	rBV	667778	1021919	30.42%	3.067%
10	7.110	693	701	712	rBV	661198	1037072	30.88%	3.112%
11	7.210	716	718	728	rVB	6120	11964	0.36%	0.036%
12	7.410	749	752	756	rVB5	3331	4086	0.12%	0.012%
13	7.569	771	779	789	rBV	623415	969012	28.85%	2.908%
14	7.810	816	820	826	rVB7	9299	17014	0.51%	0.051%
15	7.987	848	850	855	rVB5	2803	3450	0.10%	0.010%
16	8.275	892	899	910	rBV	570313	885551	26.36%	2.657%
17	8.381	914	917	920	rVB5	3203	4374	0.13%	0.013%
18	8.651	958	963	966	rBV5	3229	5410	0.16%	0.016%
19	8.710	966	973	986	rBV	660121	1049564	31.25%	3.150%
20	8.840	992	995	1001	rBV8	5185	10575	0.31%	0.032%
21	9.428	1088	1095	1105	rBV	420160	676336	20.14%	2.030%
22	9.592	1120	1123	1127	rBV5	1939	3504	0.10%	0.011%
23	9.963	1179	1186	1195	rBV	760083	1219229	36.30%	3.659%
24	10.104	1208	1210	1214	rVB5	3443	4301	0.13%	0.013%
25	10.334	1242	1249	1257	rBV	792670	1263089	37.60%	3.790%
26	10.475	1263	1273	1288	rBV	671904	1176163	35.02%	3.529%
27	11.581	1456	1461	1462	rBV4	2936	3637	0.11%	0.011%
28	11.928	1516	1520	1529	rVB4	6977	14785	0.44%	0.044%
29	12.328	1584	1588	1591	rBV4	2248	3664	0.11%	0.011%
30	13.180	1728	1733	1737	rVB5	2578	3361	0.10%	0.010%
31	13.627	1803	1809	1819	rBV	1269325	1708531	50.87%	5.127%
32	13.892	1847	1854	1865	rBV	1483028	2116599	63.01%	6.352%
33	14.204	1899	1907	1916	rBV	1102451	1513388	45.06%	4.541%
34	14.416	1936	1943	1956	rBV	73412	155830	4.64%	0.468%
35	14.622	1975	1978	1985	rBV9	2242	4135	0.12%	0.012%
36	15.045	2046	2050	2054	rBV5	6174	9252	0.28%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048990.D
 Acq On : 13 Dec 2024 20:16
 Operator : RC/JU
 Sample : P5247-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7T2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

37	15.204	2069	2077	2087	rBV	2017270	2691045	80.12%	8.075%
38	15.321	2091	2097	2113	rVV	377331	507258	15.10%	1.522%
39	15.439	2115	2117	2122	rVB3	5361	7652	0.23%	0.023%
40	16.733	2335	2337	2345	rVB4	5248	7405	0.22%	0.022%
41	16.951	2368	2374	2383	rBV	1259700	1642116	48.89%	4.928%
42	17.051	2385	2391	2403	rVB	2347591	2980827	88.74%	8.945%
43	17.339	2436	2440	2443	rBV6	2980	4082	0.12%	0.012%
44	17.662	2491	2495	2500	rVB8	3666	5188	0.15%	0.016%
45	17.874	2527	2531	2534	rBV5	7634	10274	0.31%	0.031%
46	17.945	2539	2543	2544	rBV4	3638	4073	0.12%	0.012%
47	18.821	2687	2692	2694	rVB6	2958	4153	0.12%	0.012%
48	18.915	2704	2708	2713	rBV4	20678	25876	0.77%	0.078%
49	18.986	2715	2720	2725	rBV3	17434	23896	0.71%	0.072%
50	19.039	2725	2729	2735	rBV5	23681	37983	1.13%	0.114%
51	19.162	2748	2750	2753	rVB4	6369	6166	0.18%	0.019%
52	19.351	2776	2782	2789	rBV	2645756	3358912	100.00%	10.080%
53	19.592	2821	2823	2826	rBV4	5344	8050	0.24%	0.024%
54	20.168	2919	2921	2922	rBV	6953	5006	0.15%	0.015%
55	21.174	3086	3092	3100	rBV	1210835	1621970	48.29%	4.867%
56	23.792	3529	3537	3551	rBV	1402406	2965911	88.30%	8.900%
57	23.980	3561	3569	3578	rBV	755194	1662604	49.50%	4.989%




Sum of corrected areas: 33323875

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048990.D
Acq On : 13 Dec 2024 20:16
Operator : RC/JU
Sample : P5247-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7T2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

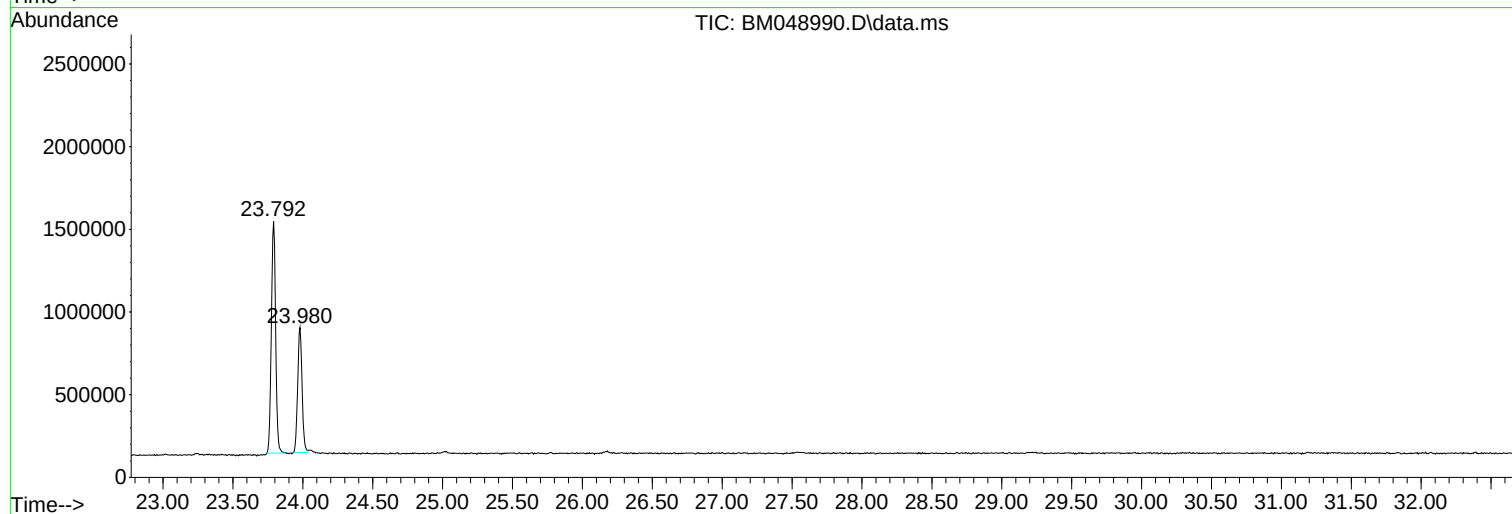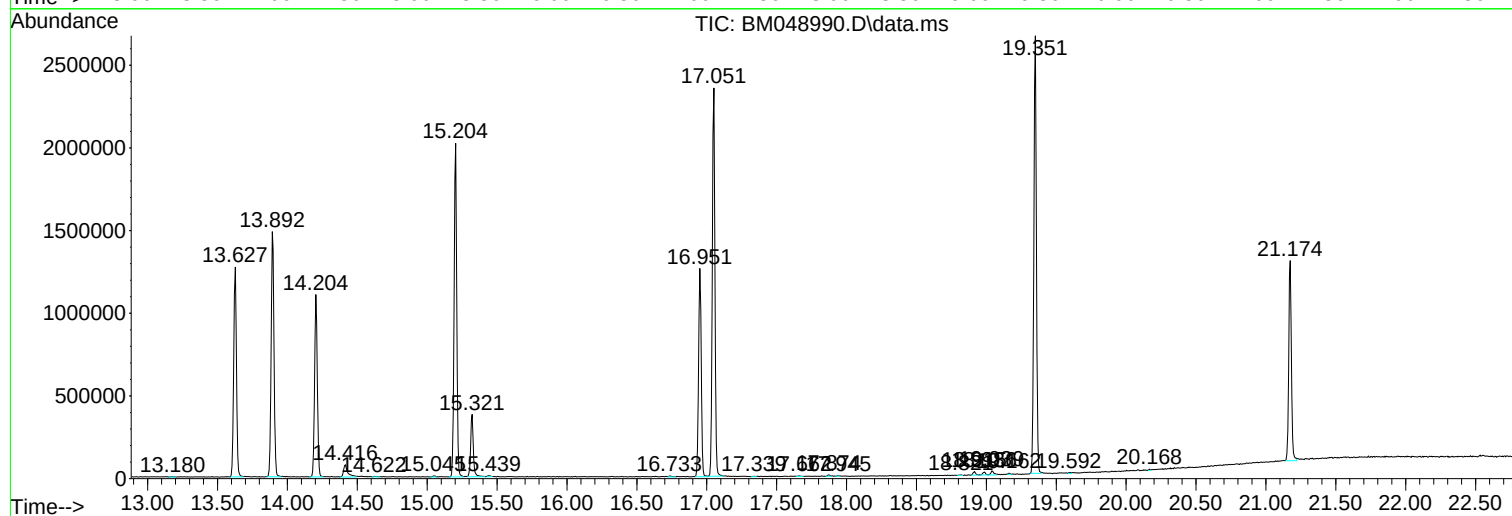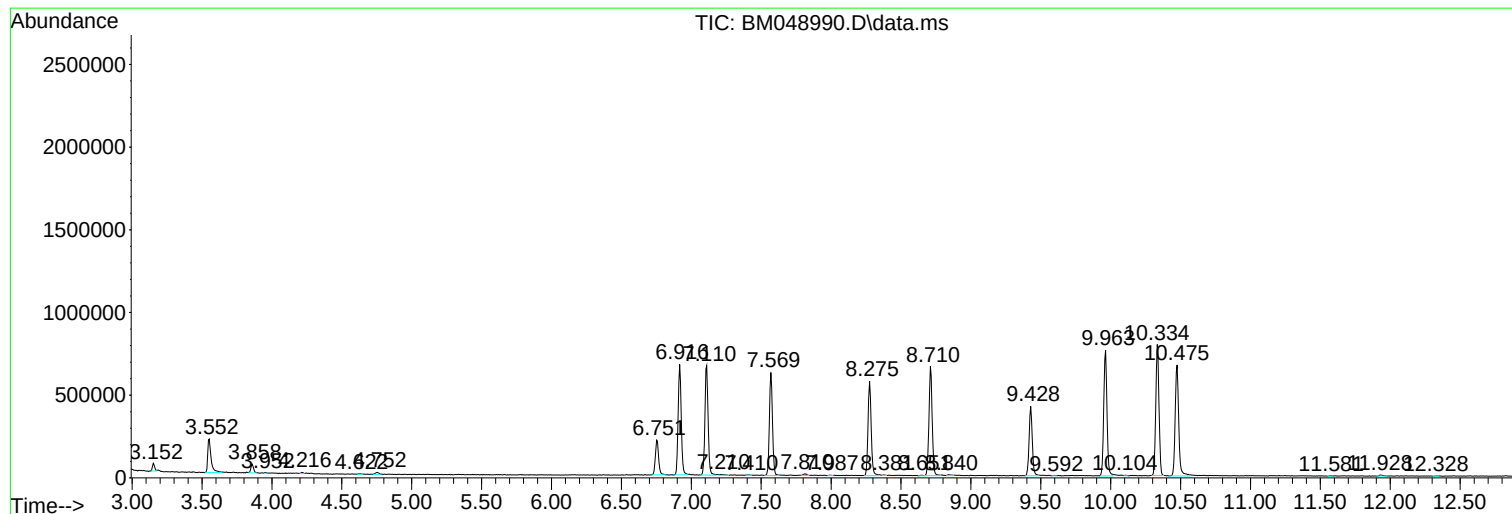

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048990.D
Acq On : 13 Dec 2024 20:16
Operator : RC/JU
Sample : P5247-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7T2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048990.D
Acq On : 13 Dec 2024 20:16
Operator : RC/JU
Sample : P5247-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7T2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------