

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
 Data File : BM048991.D
 Acq On : 13 Dec 2024 20:55
 Operator : RC/JU
 Sample : P5247-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7T5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048991.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	25	28	32	rBV	47182	55050	1.57%	0.155%
2	3.552	92	96	113	rBV	145631	252617	7.20%	0.711%
3	3.858	143	148	161	rVB	2273930	2877070	82.03%	8.102%
4	4.216	207	209	212	rVB3	5933	5142	0.15%	0.014%
5	4.563	266	268	271	rBV4	3663	4284	0.12%	0.012%
6	4.634	276	280	282	rVB5	4251	6061	0.17%	0.017%
7	4.752	295	300	303	rBV6	5809	9399	0.27%	0.026%
8	6.751	633	640	649	rBV	180596	293916	8.38%	0.828%
9	6.916	662	668	678	rBV	665725	1010833	28.82%	2.847%
10	7.110	693	701	710	rBV	644416	998680	28.47%	2.813%
11	7.216	716	719	724	rVB7	3187	5620	0.16%	0.016%
12	7.569	773	779	788	rVB	630244	951134	27.12%	2.679%
13	7.816	815	821	826	rBV7	10157	19709	0.56%	0.056%
14	8.275	892	899	909	rBV	516893	803908	22.92%	2.264%
15	8.710	966	973	984	rBV	635707	1020441	29.10%	2.874%
16	9.428	1086	1095	1107	rBV	415104	661101	18.85%	1.862%
17	9.963	1179	1186	1201	rBV	724473	1185637	33.81%	3.339%
18	10.128	1212	1214	1217	rVB4	4047	3627	0.10%	0.010%
19	10.334	1242	1249	1258	rBV	780241	1262664	36.00%	3.556%
20	10.475	1265	1273	1283	rBV	495939	871761	24.86%	2.455%
21	11.933	1517	1521	1526	rBV4	7687	13058	0.37%	0.037%
22	12.563	1624	1628	1633	rBV6	3221	5193	0.15%	0.015%
23	12.822	1669	1672	1677	rVB7	2854	3816	0.11%	0.011%
24	13.628	1802	1809	1816	rBV	1267209	1703155	48.56%	4.796%
25	13.892	1847	1854	1865	rBV	1486583	2065446	58.89%	5.817%
26	14.204	1900	1907	1915	rBV	1070943	1487204	42.40%	4.188%
27	14.416	1937	1943	1954	rBV	61783	132876	3.79%	0.374%
28	14.486	1954	1955	1960	rVB5	3727	4537	0.13%	0.013%
29	14.639	1975	1981	1985	rBV6	5231	5942	0.17%	0.017%
30	15.051	2047	2051	2054	rBV3	5389	8257	0.24%	0.023%
31	15.204	2070	2077	2088	rBV	1963730	2656577	75.75%	7.482%
32	15.322	2090	2097	2103	rBV	381204	501346	14.29%	1.412%
33	15.439	2113	2117	2122	rVB5	6921	10563	0.30%	0.030%
34	15.586	2138	2142	2145	rBV4	2882	3650	0.10%	0.010%
35	16.745	2334	2339	2344	rVB5	4795	7966	0.23%	0.022%
36	16.845	2351	2356	2358	rBV3	2185	3959	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048991.D
Acq On : 13 Dec 2024 20:55
Operator : RC/JU
Sample : P5247-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7T5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Title : SVOA CALIBRATION

37	16.951	2366	2374	2381	rBV2	1179595	1607361	45.83%	4.527%
38	17.051	2384	2391	2404	rBV	2264282	2989858	85.25%	8.420%
39	17.868	2526	2530	2536	rBV6	10259	17906	0.51%	0.050%
40	17.939	2538	2542	2544	rBV4	4322	4748	0.14%	0.013%
41	18.651	2658	2663	2664	rBV5	2881	3602	0.10%	0.010%
42	18.915	2703	2708	2712	rBV3	19027	26461	0.75%	0.075%
43	18.980	2715	2719	2725	rBV2	19121	25036	0.71%	0.071%
44	19.039	2725	2729	2737	rBV5	39771	65446	1.87%	0.184%
45	19.162	2747	2750	2755	rVB7	8659	11659	0.33%	0.033%
46	19.351	2775	2782	2791	rBV	2761380	3507227	100.00%	9.877%
47	19.762	2850	2852	2854	rBV3	5170	4873	0.14%	0.014%
48	21.174	3086	3092	3100	rBV	1197588	1624285	46.31%	4.574%
49	23.786	3529	3536	3548	rBV	1394867	3050500	86.98%	8.591%
50	23.980	3561	3569	3578	rBV	736765	1657319	47.25%	4.667%




Sum of corrected areas: 35508480

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048991.D
Acq On : 13 Dec 2024 20:55
Operator : RC/JU
Sample : P5247-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7T5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

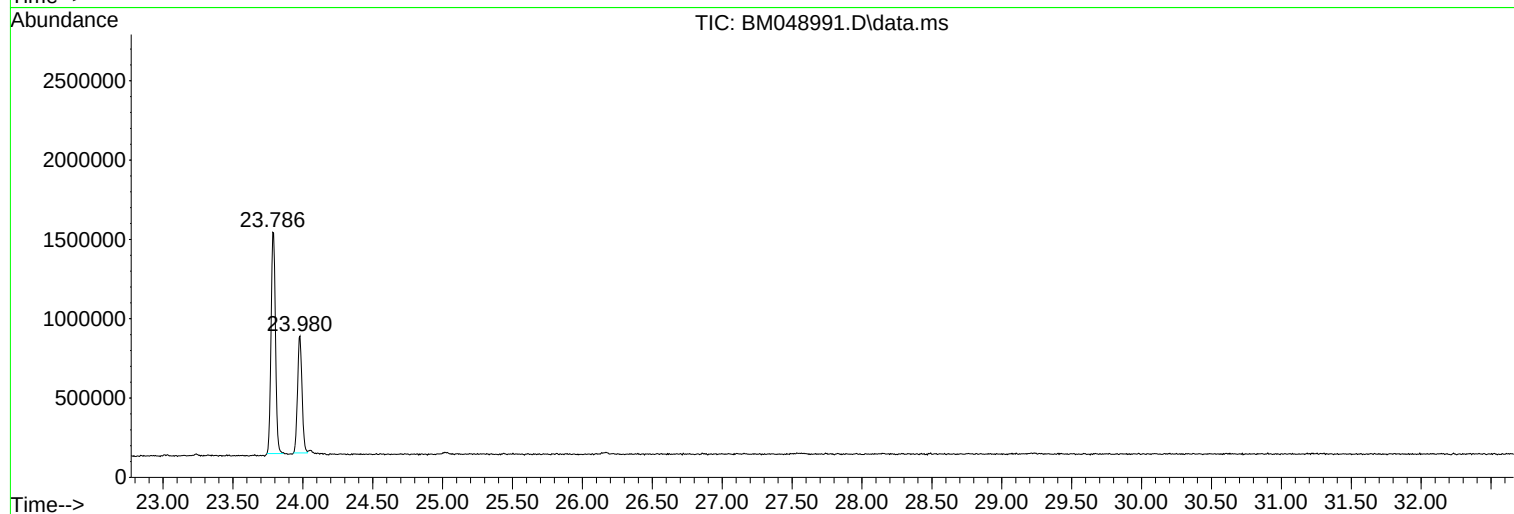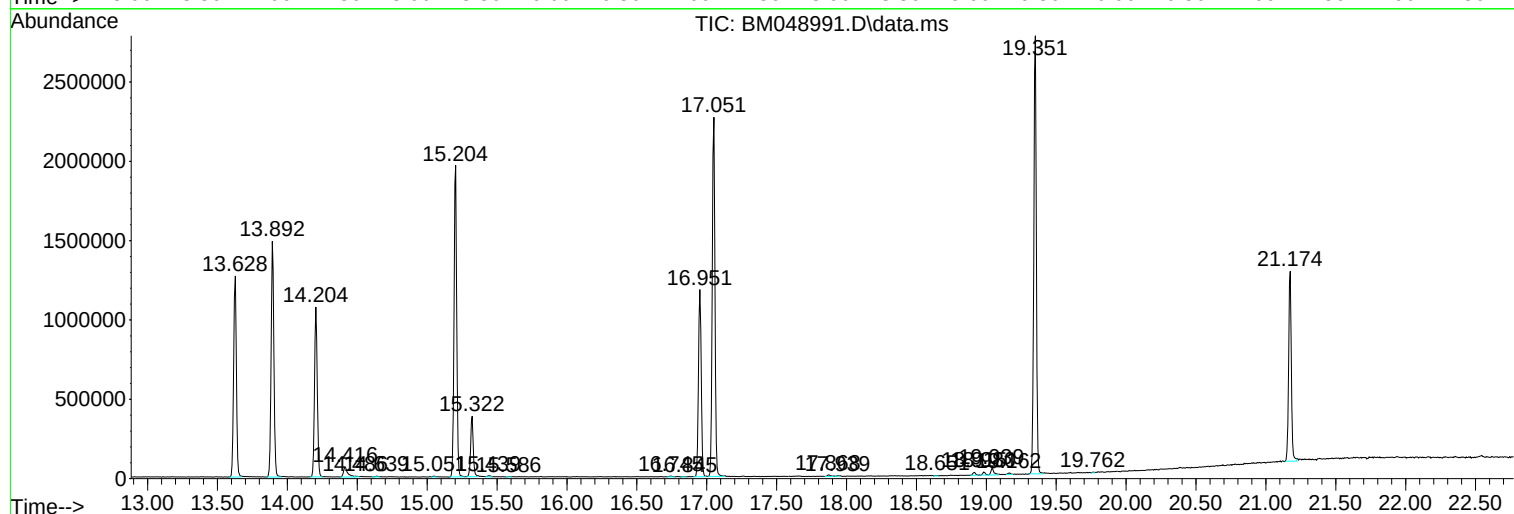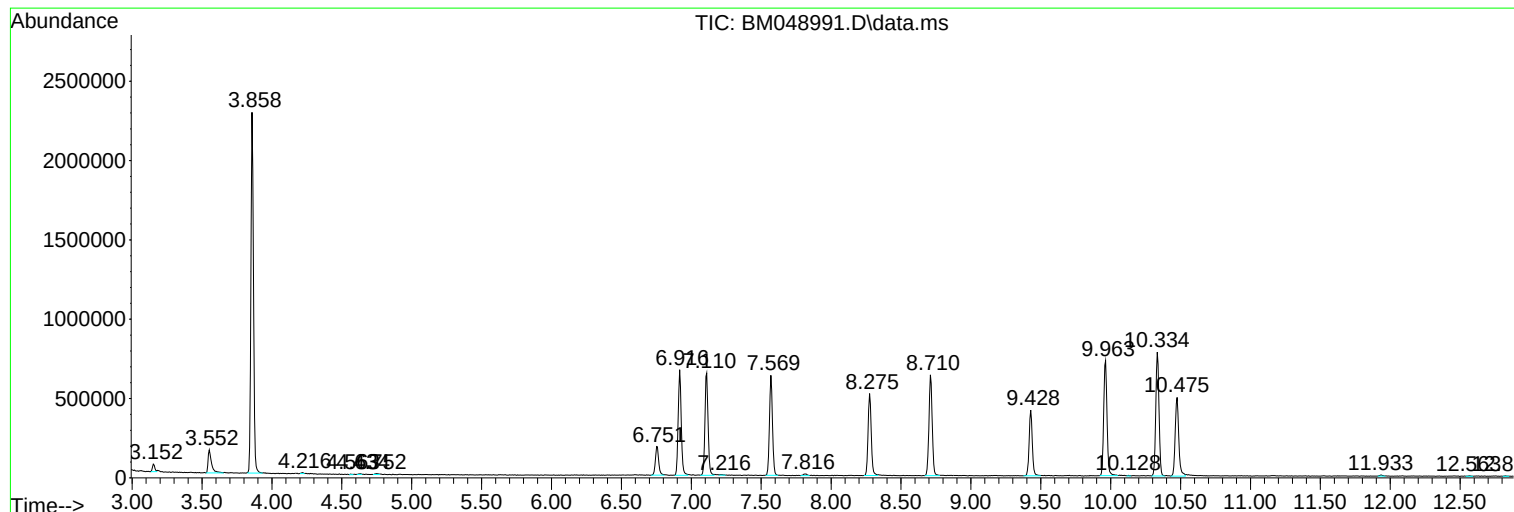

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048991.D
Acq On : 13 Dec 2024 20:55
Operator : RC/JU
Sample : P5247-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7T5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121324\
Data File : BM048991.D
Acq On : 13 Dec 2024 20:55
Operator : RC/JU
Sample : P5247-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7T5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc