

Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM121415\  
 Data File : BM003540.D  
 Acq On : 14 Dec 2015 14:42  
 Operator : UM/IZ  
 Sample : G4722-16  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C04D6

Quant Time: Dec 15 00:21:58 2015  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM02.2-EPA-BM120115.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 15 00:18:50 2015  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.72  | 152  | 76001    | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.51 | 136  | 351133   | 20.00 | ng/ul | 0.00     |
| 36) Acenaphthene-d10      | 14.37 | 164  | 194368   | 20.00 | ng/ul | 0.00     |
| 62) Phenanthrene-d10      | 17.12 | 188  | 392895   | 20.00 | ng/ul | 0.00     |
| 78) Chrysene-d12          | 21.32 | 240  | 343567   | 20.00 | ng/ul | 0.00     |
| 86) Perylene-d12          | 23.57 | 264  | 326193   | 20.00 | ng/ul | -0.01    |

| System Monitoring Compounds    | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|--------------------------------|-------|------|----------|-------|-------|----------|
| 3) 1,4-Dioxane-d8              | 3.18  | 96   | 2257     | 1.48  | ng/uL | 0.00     |
| 5) Phenol-d5                   | 6.90  | 99   | 52828    | 8.71  | ng/ul | 0.00     |
| 7) Bis-(2-Chloroethyl)ether-d  | 7.05  | 67   | 118359   | 35.36 | ng/ul | 0.00     |
| 9) 2-Chlorophenol-d4           | 7.25  | 132  | 155310   | 30.96 | ng/ul | 0.00     |
| 13) 4-Methylphenol-d8          | 8.43  | 113  | 104011   | 20.43 | ng/ul | 0.00     |
| 19) Nitrobenzene-d5            | 8.88  | 128  | 92810    | 38.75 | ng/ul | 0.00     |
| 22) 2-Nitrophenol-d4           | 9.60  | 143  | 103481   | 41.33 | ng/ul | 0.00     |
| 26) 2,4-Dichlorophenol-d3      | 10.13 | 165  | 177989   | 35.85 | ng/ul | 0.00     |
| 29) 4-Chloroaniline-d4         | 10.65 | 131  | 243771   | 43.39 | ng/ul | 0.00     |
| 44) Dimethylphthalate-d6       | 13.78 | 166  | 581601   | 39.80 | ng/ul | 0.00     |
| 47) Acenaphthylene-d8          | 14.06 | 160  | 689627   | 38.39 | ng/ul | 0.00     |
| 52) 4-Nitrophenol-d4           | 14.59 | 143  | 12602    | 4.81  | ng/ul | 0.00     |
| 58) Fluorene-d10               | 15.37 | 176  | 490933   | 39.04 | ng/ul | 0.00     |
| 63) 4,6-Dinitro-2-methylphenol | 15.49 | 200  | 57773    | 28.74 | ng/ul | 0.00     |
| 71) Anthracene-d10             | 17.22 | 188  | 681078   | 39.02 | ng/ul | 0.00     |
| 79) Pyrene-d10                 | 19.52 | 212  | 684719   | 40.71 | ng/ul | 0.00     |
| 90) Benzo(a)pyrene-d12         | 23.43 | 264  | 564030   | 35.84 | ng/ul | -0.01    |


| Target Compounds       | R.T.  | QIon | Response | Conc | Units  | Qvalue |
|------------------------|-------|------|----------|------|--------|--------|
| 46) 2,6-Dinitrotoluene | 13.79 | 165  | 3530     | 1.28 | ng/ul# | 37     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM121415\  
Data File : BM003540.D  
Acq On : 14 Dec 2015 14:42  
Operator : UM/IZ  
Sample : G4722-16  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
C04D6

Quant Time: Dec 15 00:21:58 2015  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM02.2-EPA-BM120115.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Dec 15 00:18:50 2015  
Response via : Initial Calibration

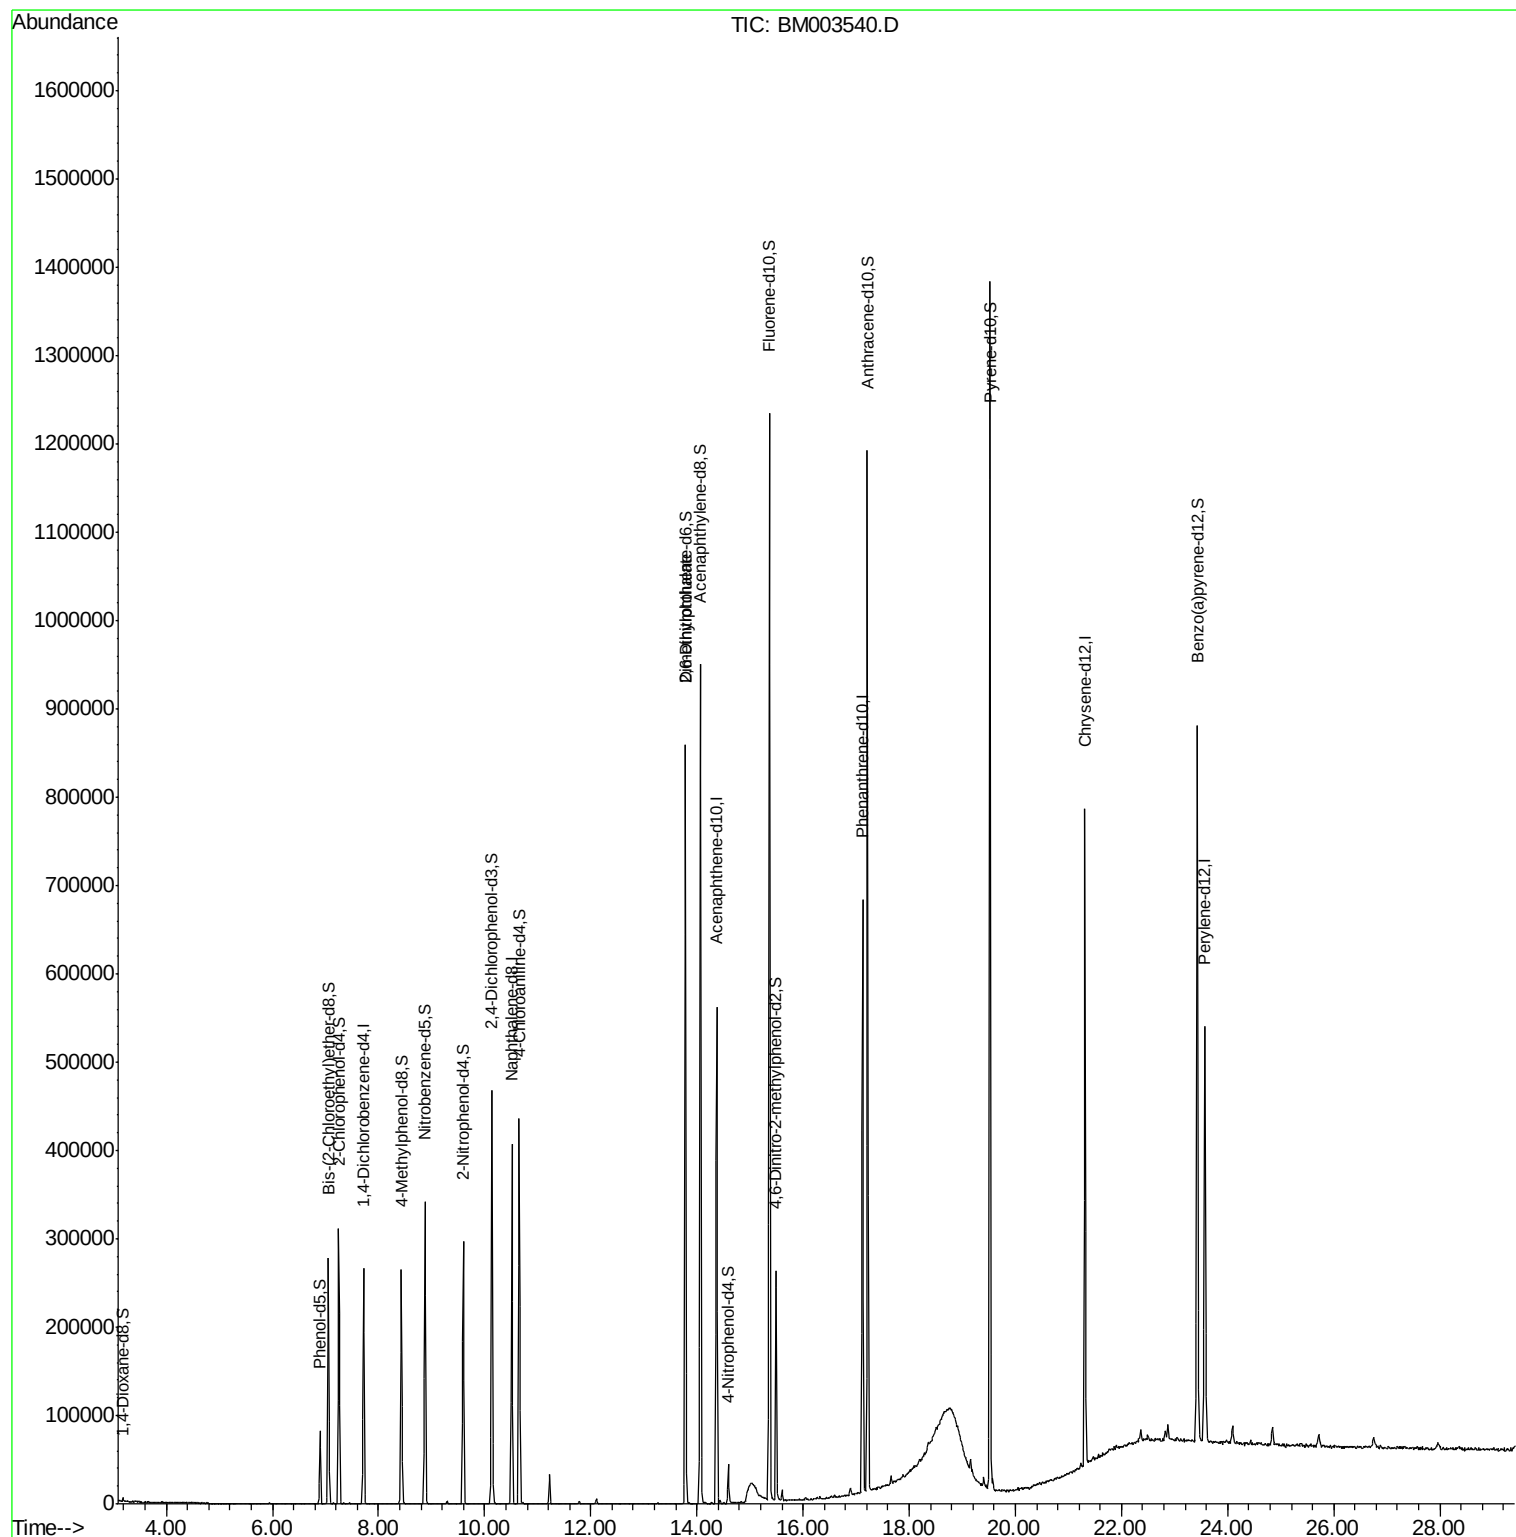

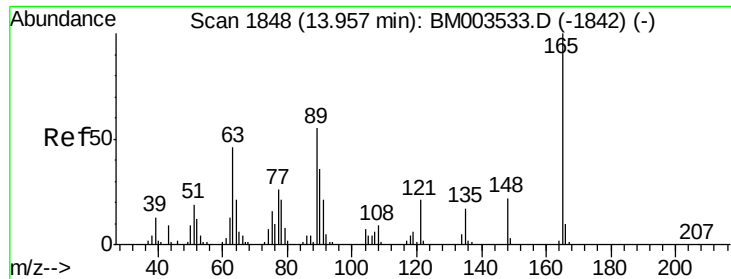

#46

2,6-Dinitrotoluene

Concen: 1.28 ng/ul

RT: 13.79 min Scan# 1819

Delta R.T. -0.17 min

Lab File: BM003540.D


Acq: 14 Dec 2015 14:42

Instrument :

BNA\_M

ClientSampleId :

C04D6

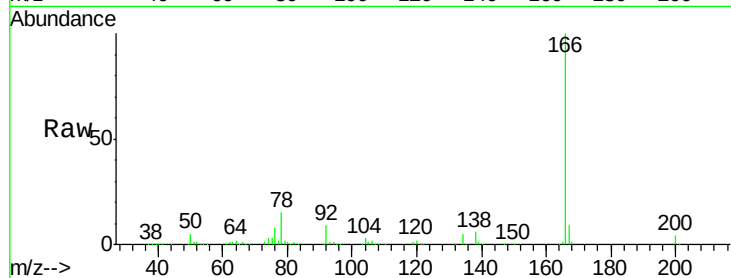

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 165   | Resp: | 3530  |
| Ion Ratio | Lower | Upper |       |
| 165       | 100   |       |       |
| 89        | 0.0   | 42.0  | 63.0# |
| 121       | 35.9  | 16.6  | 24.8# |

