

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
 Data File : BM003542.D
 Acq On : 14 Dec 2015 15:55
 Operator : UM/IZ
 Sample : G4722-18
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04D8

Quant Time: Dec 15 00:22:19 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 15 00:18:50 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	72849	20.00	ng/ul	0.00
18) Naphthalene-d8	10.51	136	342140	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.37	164	194122	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.12	188	387798	20.00	ng/ul	0.00
78) Chrysene-d12	21.32	240	331664	20.00	ng/ul	0.00
86) Perylene-d12	23.57	264	311381	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	1405	0.96	ng/uL	0.00
5) Phenol-d5	6.90	99	36984	6.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	80084	24.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	105690	21.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.43	113	71771	14.71	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	62570	26.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	68238	27.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	121667	25.15	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	138401	25.28	ng/ul	0.00
44) Dimethylphthalate-d6	13.78	166	402967	27.61	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	466604	26.01	ng/ul	0.00
52) 4-Nitrophenol-d4	14.59	143	8155	3.12	ng/ul	0.00
58) Fluorene-d10	15.37	176	321965	25.64	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.49	200	30358	15.30	ng/ul	0.00
71) Anthracene-d10	17.22	188	438335	25.44	ng/ul	0.00
79) Pyrene-d10	19.52	212	445588	27.44	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.43	264	329215	21.91	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.83	163	53881	3.59	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003542.D
Acq On : 14 Dec 2015 15:55
Operator : UM/IZ
Sample : G4722-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04D8

Quant Time: Dec 15 00:22:19 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 15 00:18:50 2015
Response via : Initial Calibration

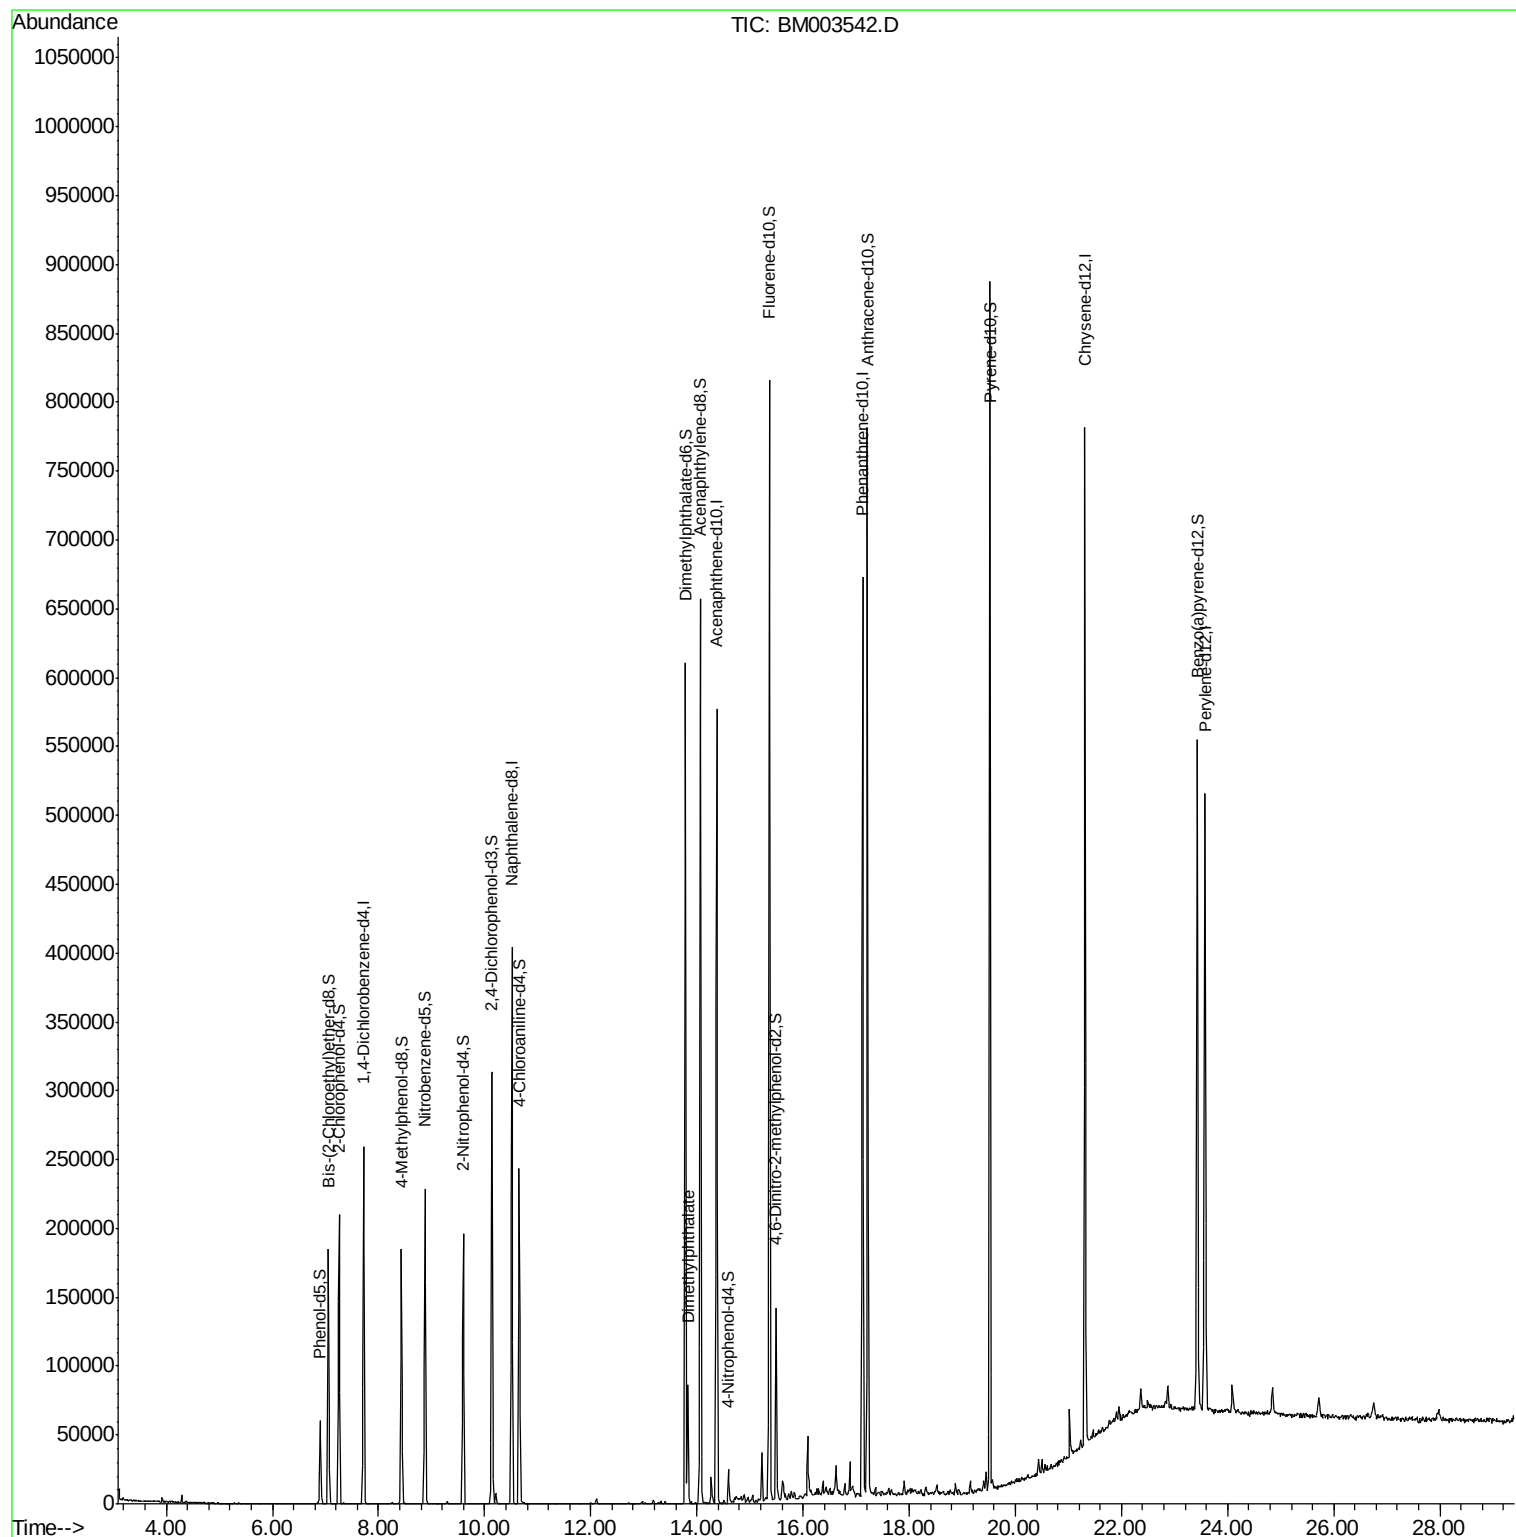

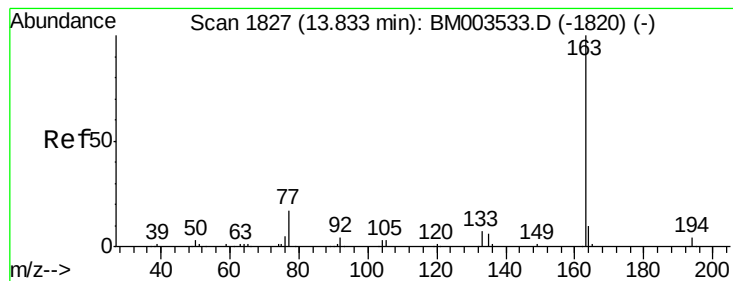

#45

Dimethylphthalate

Concen: 3.59 ng/ul

RT: 13.83 min Scan# 1826

Delta R.T. -0.01 min

Lab File: BM003542.D


Acq: 14 Dec 2015 15:55

Instrument :

BNA_M

ClientSampleId :

C04D8

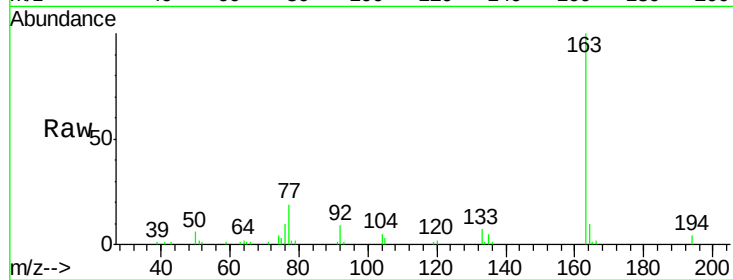


Tgt Ion:163 Resp: 53881

Ion Ratio Lower Upper

163 100

194 3.6 3.2 4.8

164 10.1 8.3 12.5

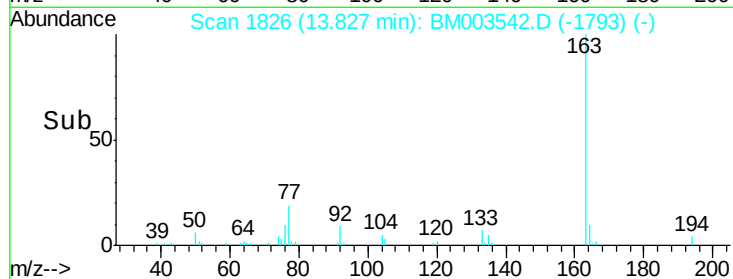

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

