

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
 Data File : BM003536.D
 Acq On : 14 Dec 2015 12:17
 Operator : UM/IZ
 Sample : G4722-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04C6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	21	rVB	4036	4814	0.22%	0.025%
2	3.922	138	142	147	rVB2	1801	2622	0.12%	0.013%
3	5.769	453	456	460	rBB	3164	3568	0.16%	0.018%
4	6.857	637	641	642	rBV	3963	4582	0.21%	0.023%
5	6.892	642	647	655	rVB	85315	128795	5.89%	0.656%
6	7.051	668	674	685	rBB	301051	462715	21.17%	2.358%
7	7.251	702	708	717	rBB	336336	519644	23.78%	2.648%
8	7.716	781	787	795	rBB	269862	429649	19.66%	2.189%
9	8.428	902	908	917	rBB	274216	421285	19.28%	2.147%
10	8.875	977	984	996	rBB	373019	604838	27.68%	3.082%
11	9.292	1051	1055	1059	rBB2	2548	3824	0.17%	0.019%
12	9.598	1100	1107	1114	rBB	319950	512285	23.44%	2.610%
13	9.922	1158	1162	1166	rBB	6612	8280	0.38%	0.042%
14	10.133	1191	1198	1209	rBV	496298	806367	36.90%	4.109%
15	10.510	1255	1262	1271	rBB	422113	691903	31.66%	3.526%
16	10.651	1281	1286	1293	rBB2	15022	23923	1.09%	0.122%
17	12.104	1529	1533	1537	rBB2	5948	9182	0.42%	0.047%
18	12.968	1678	1680	1683	rBB	2355	2435	0.11%	0.012%
19	13.780	1812	1818	1830	rBV	891555	1243789	56.91%	6.338%
20	14.063	1859	1866	1889	rBV	1044570	1533374	70.16%	7.813%
21	14.374	1912	1919	1927	rBV2	592412	931937	42.64%	4.749%
22	14.586	1950	1955	1964	rBV	41107	64459	2.95%	0.328%
23	15.368	2081	2088	2096	rBV	1307535	1904319	87.14%	9.704%
24	15.486	2103	2108	2119	rVB	323608	448059	20.50%	2.283%
25	15.604	2125	2128	2132	rVB	11968	14519	0.66%	0.074%
26	15.762	2151	2155	2160	rBV	9907	13279	0.61%	0.068%
27	15.974	2187	2191	2195	rBB	11374	12327	0.56%	0.063%
28	16.204	2227	2230	2235	rBB	2114	2746	0.13%	0.014%
29	16.262	2236	2240	2245	rBB2	6606	9187	0.42%	0.047%
30	16.321	2246	2250	2256	rBB2	2521	3258	0.15%	0.017%
31	16.533	2281	2286	2288	rBB2	1838	2719	0.12%	0.014%
32	16.598	2292	2297	2301	rBV2	2779	4373	0.20%	0.022%
33	16.821	2330	2335	2338	rBV	6089	9360	0.43%	0.048%
34	16.856	2338	2341	2345	rVV3	4084	5462	0.25%	0.028%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
Data File : BM003536.D
Acq On : 14 Dec 2015 12:17
Operator : UM/IZ
Sample : G4722-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION

35	16.904	2345	2349	2355	rVB	2416	4200	0.19%	0.021%
36	16.998	2360	2365	2369	rVB2	2050	3427	0.16%	0.017%
37	17.121	2379	2386	2396	rBV2	741438	1097951	50.24%	5.595%
38	17.215	2396	2402	2414	rVV2	1293198	1962083	89.78%	9.998%
39	17.403	2431	2434	2439	rVB	1892	2974	0.14%	0.015%
40	17.456	2439	2443	2447	rBV	2920	4559	0.21%	0.023%
41	17.951	2524	2527	2531	rBV2	1309	2390	0.11%	0.012%
42	18.086	2546	2550	2554	rVB	6449	7834	0.36%	0.040%
43	18.350	2590	2595	2601	rBV3	4476	7437	0.34%	0.038%
44	18.427	2607	2608	2614	rVB3	3297	2835	0.13%	0.014%
45	18.503	2618	2621	2622	rBV2	3709	4020	0.18%	0.020%
46	18.521	2622	2624	2628	rVB2	5132	5518	0.25%	0.028%
47	19.086	2715	2720	2721	rBV5	2157	3267	0.15%	0.017%
48	19.150	2726	2731	2735	rVB2	15799	23283	1.07%	0.119%
49	19.403	2770	2774	2779	rBV	14024	18303	0.84%	0.093%
50	19.450	2779	2782	2786	rVB	8662	11638	0.53%	0.059%
51	19.521	2787	2794	2800	rBV	1577951	2185435	100.00%	11.136%
52	19.792	2838	2840	2841	rBV2	4121	2372	0.11%	0.012%
53	20.115	2893	2895	2900	rBV4	4750	8389	0.38%	0.043%
54	21.315	3094	3099	3107	rBV	824486	1058851	48.45%	5.396%
55	23.427	3451	3458	3470	rVB	758097	1452729	66.47%	7.403%
56	23.574	3476	3483	3494	rVB	472215	911303	41.70%	4.644%


Sum of corrected areas: 19624676

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
Data File : BM003536.D
Acq On : 14 Dec 2015 12:17
Operator : UM/IZ
Sample : G4722-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C6

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

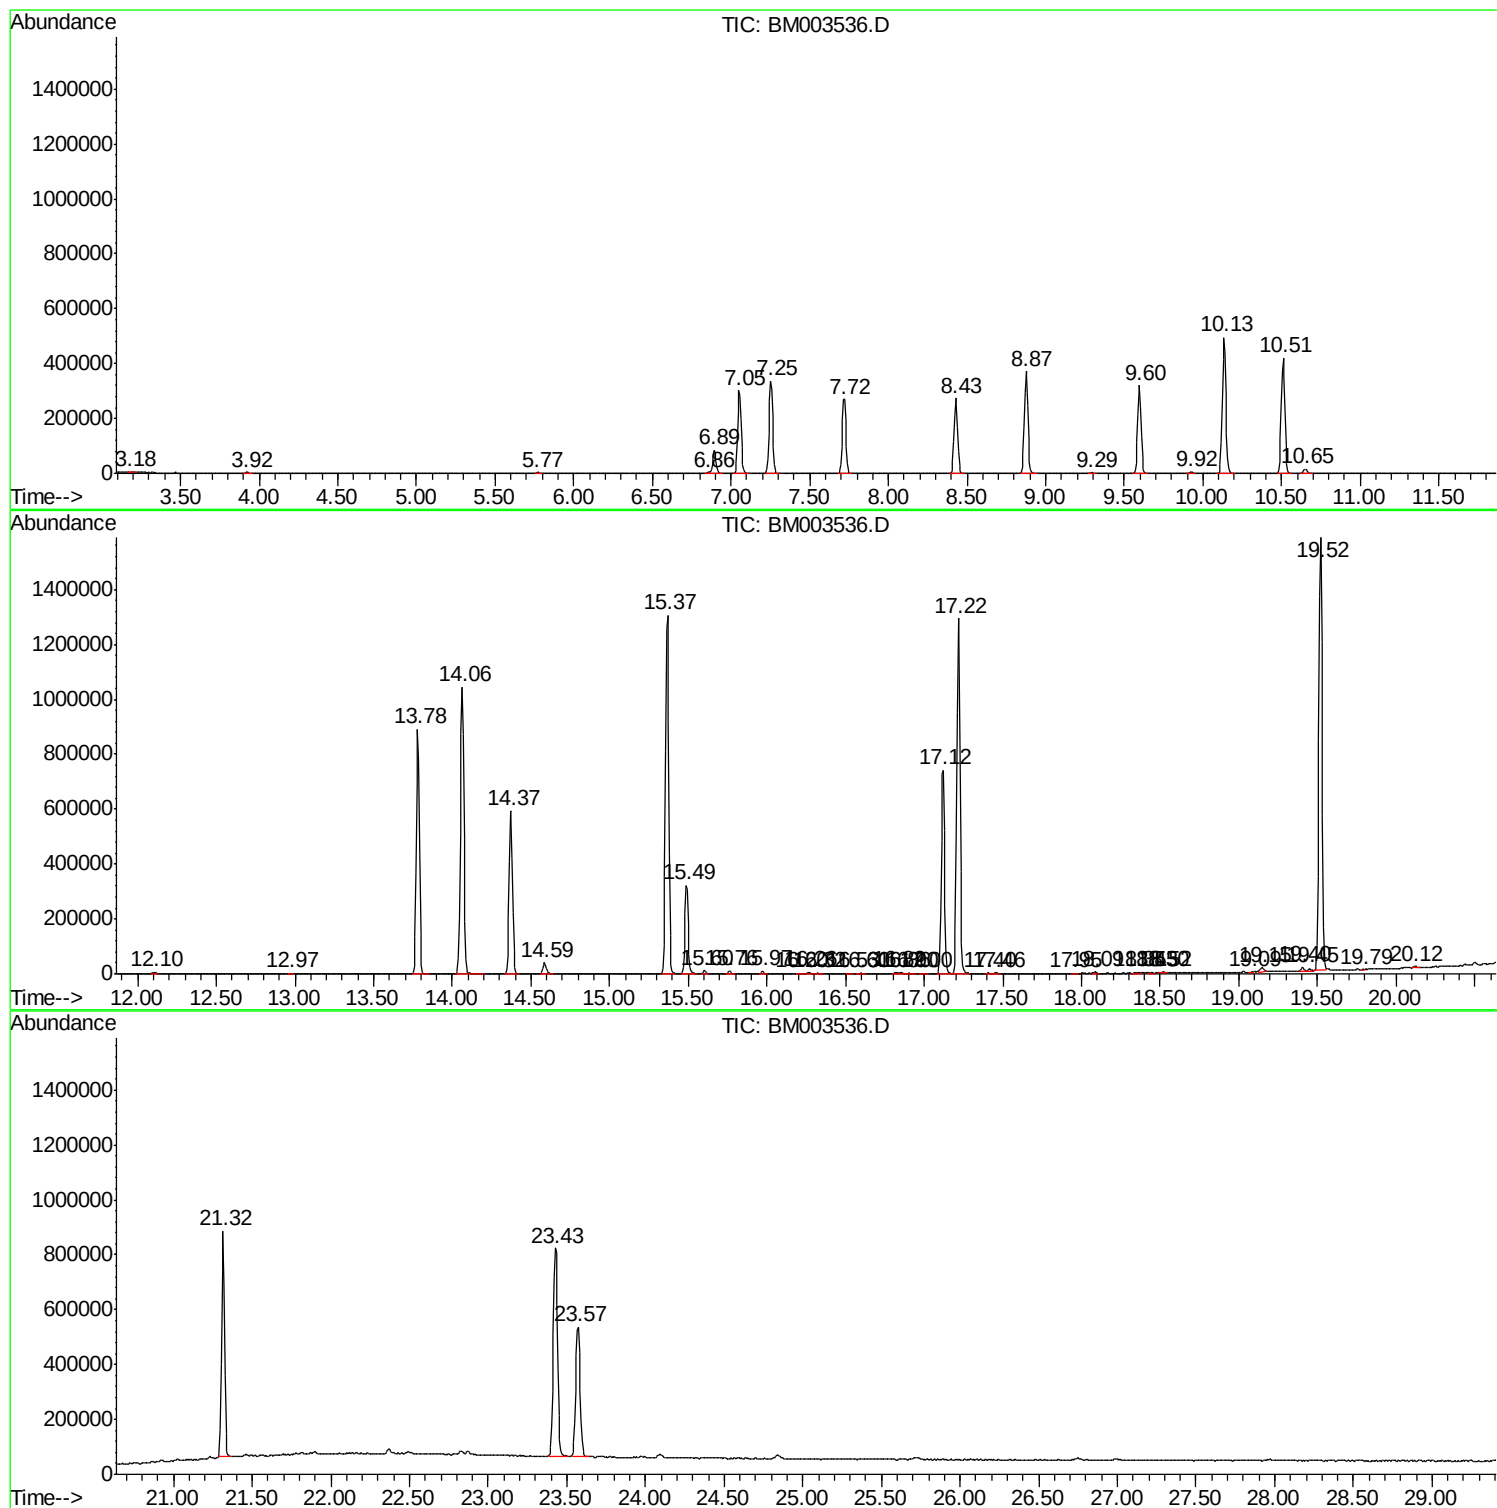

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003536.D
Acq On : 14 Dec 2015 12:17
Operator : UM/IZ
Sample : G4722-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003536.D
Acq On : 14 Dec 2015 12:17
Operator : UM/IZ
Sample : G4722-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc