

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
 Data File : BM003537.D
 Acq On : 14 Dec 2015 12:53
 Operator : UM/IZ
 Sample : G4722-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04D2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	20	rBV	4748	6246	0.30%	0.029%
2	3.222	20	23	29	rVB3	2776	3867	0.19%	0.018%
3	3.916	139	141	146	rVB	2108	2601	0.12%	0.012%
4	4.381	214	220	226	rBV	1547	3447	0.17%	0.016%
5	5.046	328	333	336	rVB	3386	4990	0.24%	0.023%
6	5.740	447	451	454	rBB	1774	2345	0.11%	0.011%
7	6.893	638	647	666	rBV2	113779	227120	10.89%	1.062%
8	7.051	668	674	687	rBB	340131	529881	25.41%	2.478%
9	7.251	702	708	716	rBV	407036	628030	30.11%	2.937%
10	7.722	781	788	794	rBB	298582	478077	22.92%	2.236%
11	8.110	850	854	859	rBB	1735	2667	0.13%	0.012%
12	8.228	870	874	879	rBB2	7127	10728	0.51%	0.050%
13	8.428	902	908	919	rBB	330844	529863	25.41%	2.478%
14	8.775	963	967	970	rBB2	2182	2849	0.14%	0.013%
15	8.875	977	984	994	rBB	420162	683737	32.78%	3.198%
16	8.951	994	997	1000	rBV	2120	2686	0.13%	0.013%
17	9.598	1100	1107	1114	rBB	358953	589448	28.26%	2.757%
18	9.922	1157	1162	1168	rBB	23357	35865	1.72%	0.168%
19	10.051	1181	1184	1188	rBB2	2243	3032	0.15%	0.014%
20	10.134	1191	1198	1211	rBV	564286	913938	43.82%	4.274%
21	10.510	1255	1262	1269	rBV	457443	761470	36.51%	3.561%
22	10.651	1278	1286	1294	rBB3	11264	21053	1.01%	0.098%
23	11.086	1356	1360	1364	rBB2	2491	3123	0.15%	0.015%
24	11.216	1379	1382	1388	rBB2	2702	4424	0.21%	0.021%
25	11.316	1395	1399	1400	rBV2	1794	2209	0.11%	0.010%
26	11.357	1401	1406	1410	rVB2	2138	4213	0.20%	0.020%
27	11.639	1448	1454	1457	rVB	1760	3161	0.15%	0.015%
28	11.722	1464	1468	1471	rBV2	3659	6088	0.29%	0.028%
29	11.757	1471	1474	1480	rVB	7789	12058	0.58%	0.056%
30	11.857	1486	1491	1499	rVB3	4199	8377	0.40%	0.039%
31	11.957	1505	1508	1513	rBV2	4080	7067	0.34%	0.033%
32	12.063	1520	1526	1527	rVV4	3130	5886	0.28%	0.028%
33	12.104	1529	1533	1537	rVB2	7308	11378	0.55%	0.053%
34	12.186	1539	1547	1552	rVV	27410	52339	2.51%	0.245%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
 Data File : BM003537.D
 Acq On : 14 Dec 2015 12:53
 Operator : UM/IZ
 Sample : G4722-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04D2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	12.233	1552	1555	1562	rVV2	11797	19783	0.95%	0.093%
36	12.298	1562	1566	1568	rVV3	2605	3310	0.16%	0.015%
37	12.333	1568	1572	1579	rVB5	3152	6149	0.29%	0.029%
38	12.433	1579	1589	1596	rBV4	11705	24338	1.17%	0.114%
39	12.563	1604	1611	1612	rBV3	4898	8136	0.39%	0.038%
40	12.651	1624	1626	1631	rVB5	2642	3791	0.18%	0.018%
41	12.745	1638	1642	1650	rBV4	12348	23510	1.13%	0.110%
42	12.892	1661	1667	1672	rBV6	5453	13585	0.65%	0.064%
43	13.033	1684	1691	1697	rBV4	11776	26296	1.26%	0.123%
44	13.086	1698	1700	1705	rVB5	2385	3840	0.18%	0.018%
45	13.227	1721	1724	1727	rVB5	3636	2918	0.14%	0.014%
46	13.263	1727	1730	1735	rVV6	2778	5731	0.27%	0.027%
47	13.310	1735	1738	1743	rVV6	6424	10649	0.51%	0.050%
48	13.375	1746	1749	1753	rVV3	3847	6971	0.33%	0.033%
49	13.427	1754	1758	1765	rVB6	7576	17510	0.84%	0.082%
50	13.551	1775	1779	1780	rBV3	2590	2733	0.13%	0.013%
51	13.592	1784	1786	1787	rBV	3795	2829	0.14%	0.013%
52	13.780	1812	1818	1828	rVB	961529	1380133	66.17%	6.454%
53	13.880	1831	1835	1838	rBV5	3519	6034	0.29%	0.028%
54	13.922	1840	1842	1848	rVB4	6275	8933	0.43%	0.042%
55	13.980	1848	1852	1855	rVB6	3652	5380	0.26%	0.025%
56	14.063	1860	1866	1876	rVB	1119251	1678323	80.47%	7.849%
57	14.157	1879	1882	1883	rBV3	2440	2220	0.11%	0.010%
58	14.186	1883	1887	1891	rBV3	7305	11669	0.56%	0.055%
59	14.292	1901	1905	1911	rBV3	14165	21140	1.01%	0.099%
60	14.374	1912	1919	1930	rVB2	626098	1003688	48.12%	4.694%
61	14.474	1930	1936	1938	rBV5	5312	6846	0.33%	0.032%
62	14.592	1950	1956	1969	rBV	69242	137183	6.58%	0.642%
63	14.739	1976	1981	1982	rBV4	9480	13308	0.64%	0.062%
64	14.863	1998	2002	2007	rVV2	14451	19477	0.93%	0.091%
65	14.916	2007	2011	2018	rVB6	16986	31739	1.52%	0.148%
66	15.369	2081	2088	2094	rBV	1411030	2037377	97.69%	9.528%
67	15.486	2103	2108	2114	rBV	366510	519978	24.93%	2.432%
68	15.604	2125	2128	2136	rVB2	19604	32289	1.55%	0.151%
69	15.886	2173	2176	2185	rVB7	8335	16071	0.77%	0.075%
70	16.204	2228	2230	2235	rBV	6076	6808	0.33%	0.032%
71	17.121	2380	2386	2394	rBV	757875	1111598	53.30%	5.199%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
Data File : BM003537.D
Acq On : 14 Dec 2015 12:53
Operator : UM/IZ
Sample : G4722-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04D2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION

72	17.221	2396	2403	2413	rVB	1376879	2045072	98.06%	9.564%
73	18.021	2536	2539	2543	rBV5	19750	30997	1.49%	0.145%
74	18.304	2585	2587	2592	rVB	19916	21954	1.05%	0.103%
75	18.486	2615	2618	2631	rVB2	36661	64525	3.09%	0.302%
76	19.521	2788	2794	2800	rBV	1497557	2085626	100.00%	9.754%
77	21.315	3095	3099	3105	rBV	711064	930701	44.62%	4.353%
78	23.433	3452	3459	3470	rVB	790053	1513683	72.58%	7.079%
79	23.574	3477	3483	3491	rVB	468641	893516	42.84%	4.179%


Sum of corrected areas: 21382610

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
Data File : BM003537.D
Acq On : 14 Dec 2015 12:53
Operator : UM/IZ
Sample : G4722-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04D2

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

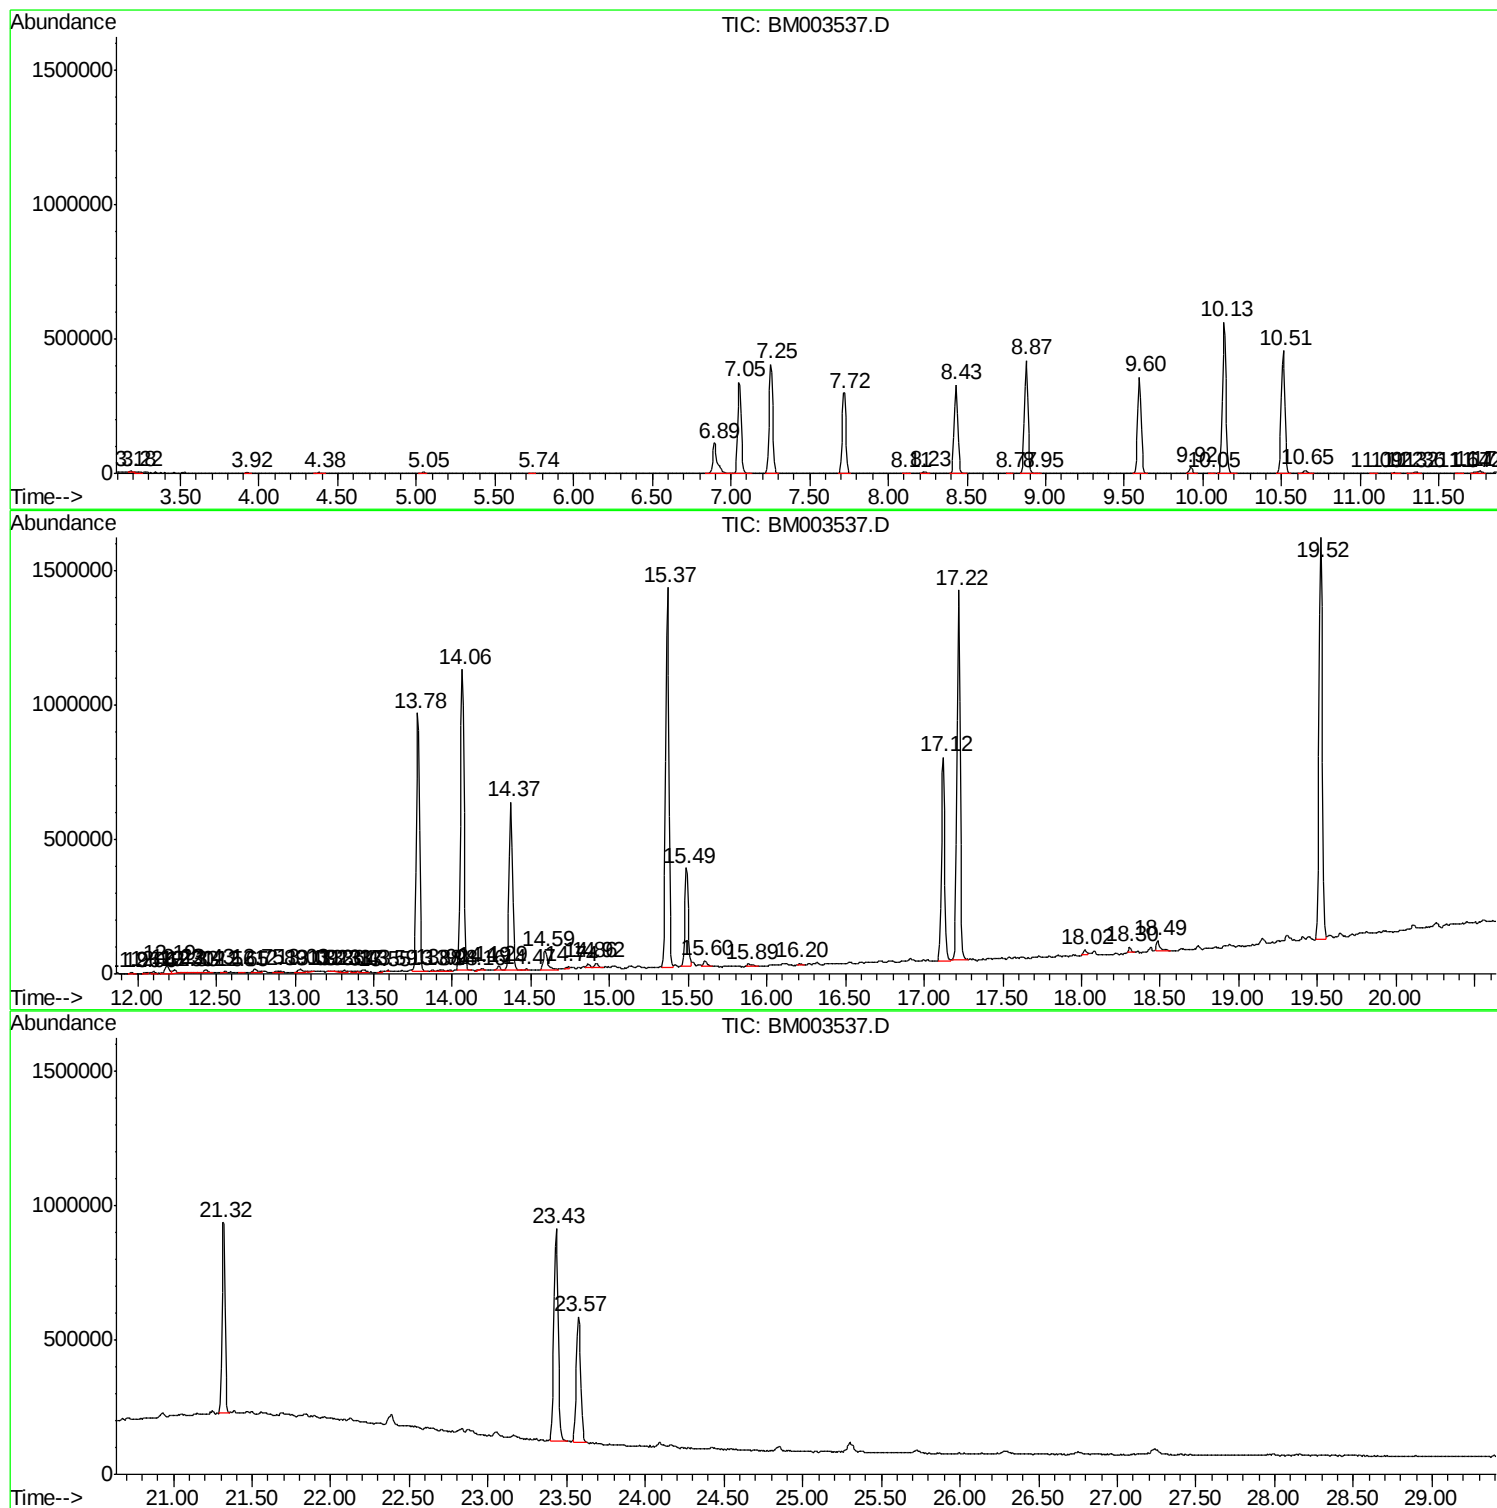

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003537.D
Acq On : 14 Dec 2015 12:53
Operator : UM/IZ
Sample : G4722-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04D2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003537.D
Acq On : 14 Dec 2015 12:53
Operator : UM/IZ
Sample : G4722-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04D2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc