

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
 Data File : BM003539.D
 Acq On : 14 Dec 2015 14:06
 Operator : UM/IZ
 Sample : G4722-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04C9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	13	17	21	rVB2	2525	3750	0.27%	0.023%
2	3.922	139	142	146	rVB	3927	5442	0.39%	0.033%
3	4.363	214	217	221	rBV3	1406	2095	0.15%	0.013%
4	6.898	641	648	657	rVB2	64002	107833	7.79%	0.662%
5	7.051	669	674	684	rBV	209088	320048	23.13%	1.964%
6	7.251	702	708	719	rVB	233599	368736	26.65%	2.263%
7	7.722	781	788	796	rVB	280755	447260	32.33%	2.745%
8	8.433	903	909	916	rBV	201529	315227	22.78%	1.935%
9	8.875	977	984	993	rVB	262473	423261	30.59%	2.598%
10	9.292	1051	1055	1059	rBB	3428	5009	0.36%	0.031%
11	9.598	1100	1107	1115	rBB	225059	360337	26.04%	2.212%
12	10.133	1192	1198	1206	rBV	353536	586413	42.39%	3.599%
13	10.210	1206	1211	1216	rVB	8865	14181	1.02%	0.087%
14	10.510	1255	1262	1272	rVB	446813	726900	52.54%	4.462%
15	10.651	1279	1286	1297	rBV	321247	533095	38.53%	3.272%
16	11.786	1473	1479	1482	rBB	1582	2429	0.18%	0.015%
17	12.010	1512	1517	1519	rBV	1235	1516	0.11%	0.009%
18	12.104	1529	1533	1539	rBB2	4071	6756	0.49%	0.041%
19	12.721	1634	1638	1642	rBV3	1258	2078	0.15%	0.013%
20	12.810	1649	1653	1658	rBB2	730	1444	0.10%	0.009%
21	12.968	1675	1680	1684	rBV2	2550	3628	0.26%	0.022%
22	13.021	1687	1689	1692	rVB	1812	1729	0.12%	0.011%
23	13.186	1714	1717	1722	rBB	3957	5392	0.39%	0.033%
24	13.263	1724	1730	1735	rBV2	1593	2934	0.21%	0.018%
25	13.316	1735	1739	1743	rVB2	3679	4992	0.36%	0.031%
26	13.404	1749	1754	1757	rBB	2523	3192	0.23%	0.020%
27	13.780	1812	1818	1823	rVV	678410	938210	67.81%	5.759%
28	13.827	1823	1826	1833	rVV	33805	45450	3.29%	0.279%
29	13.892	1835	1837	1841	rVB2	2027	2184	0.16%	0.013%
30	13.974	1846	1851	1853	rBV2	1953	2399	0.17%	0.015%
31	14.021	1855	1859	1860	rBV2	2790	2760	0.20%	0.017%
32	14.063	1860	1866	1874	rVB	750613	1072658	77.53%	6.584%
33	14.268	1895	1901	1910	rVB2	24222	41052	2.97%	0.252%
34	14.374	1910	1919	1927	rBV2	640320	990690	71.61%	6.081%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
 Data File : BM003539.D
 Acq On : 14 Dec 2015 14:06
 Operator : UM/IZ
 Sample : G4722-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04C9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	14.510	1937	1942	1948	rBV3	3461	6333	0.46%	0.039%
36	14.592	1950	1956	1965	rBV2	27951	50105	3.62%	0.308%
37	14.674	1967	1970	1973	rVB3	1918	2348	0.17%	0.014%
38	14.715	1973	1977	1978	rBV2	2962	4422	0.32%	0.027%
39	14.833	1994	1997	1999	rVB4	3141	3572	0.26%	0.022%
40	14.892	1999	2007	2011	rVB5	6226	12745	0.92%	0.078%
41	14.957	2014	2018	2022	rBV	4874	6426	0.46%	0.039%
42	15.039	2028	2032	2040	rVB6	7084	12855	0.93%	0.079%
43	15.115	2042	2045	2049	rVB6	1867	2746	0.20%	0.017%
44	15.162	2049	2053	2055	rBV3	3076	4838	0.35%	0.030%
45	15.221	2055	2063	2068	rVB	40549	53056	3.83%	0.326%
46	15.286	2068	2074	2076	rBV3	3665	6511	0.47%	0.040%
47	15.309	2076	2078	2081	rVV2	2152	2462	0.18%	0.015%
48	15.368	2081	2088	2098	rVV	914870	1337066	96.64%	8.207%
49	15.486	2103	2108	2114	rBV	167645	228094	16.49%	1.400%
50	15.615	2123	2130	2137	rBV6	16134	42334	3.06%	0.260%
51	15.668	2137	2139	2143	rVV4	4511	6287	0.45%	0.039%
52	15.727	2143	2149	2153	rVV2	5308	9702	0.70%	0.060%
53	15.780	2155	2158	2161	rVV3	6202	8181	0.59%	0.050%
54	15.839	2163	2168	2174	rVB3	5550	9642	0.70%	0.059%
55	16.051	2196	2204	2206	rBV5	3897	9304	0.67%	0.057%
56	16.086	2206	2210	2217	rVV	44283	67687	4.89%	0.415%
57	16.139	2217	2219	2221	rVB3	2511	1991	0.14%	0.012%
58	16.268	2237	2241	2243	rBV4	5159	7780	0.56%	0.048%
59	16.298	2243	2246	2252	rVB3	5024	8837	0.64%	0.054%
60	16.374	2252	2259	2262	rBV4	15386	20188	1.46%	0.124%
61	16.427	2264	2268	2274	rVV3	6893	12387	0.90%	0.076%
62	16.509	2276	2282	2285	rVV3	5545	11044	0.80%	0.068%
63	16.539	2285	2287	2291	rVV4	2571	3202	0.23%	0.020%
64	16.621	2291	2301	2307	rVV2	29677	52147	3.77%	0.320%
65	16.692	2310	2313	2317	rVB4	2466	3414	0.25%	0.021%
66	16.786	2325	2329	2334	rVB2	11372	15948	1.15%	0.098%
67	16.833	2334	2337	2338	rBV3	2387	2243	0.16%	0.014%
68	16.880	2340	2345	2348	rBV	23738	31264	2.26%	0.192%
69	16.927	2351	2353	2358	rVB3	4972	5808	0.42%	0.036%
70	17.121	2379	2386	2394	rBV	739238	1062965	76.83%	6.524%
71	17.215	2394	2402	2413	rVB2	906496	1327855	95.98%	8.150%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
Data File : BM003539.D
Acq On : 14 Dec 2015 14:06
Operator : UM/IZ
Sample : G4722-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C9

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION

72	17.362	2423	2427	2432	rVB4	7686	10761	0.78%	0.066%
73	17.480	2444	2447	2454	rVB6	4142	7502	0.54%	0.046%
74	17.615	2467	2470	2474	rBV3	4683	5067	0.37%	0.031%
75	17.798	2497	2501	2504	rBV4	2448	3500	0.25%	0.021%
76	17.909	2514	2520	2524	rBV3	10772	20306	1.47%	0.125%
77	17.968	2527	2530	2532	rBV3	3704	5001	0.36%	0.031%
78	18.015	2536	2538	2541	rVB4	7178	6931	0.50%	0.043%
79	18.315	2584	2589	2593	rBV4	5460	9874	0.71%	0.061%
80	18.433	2606	2609	2613	rVB3	2521	3325	0.24%	0.020%
81	18.503	2620	2621	2622	rBV	3181	1902	0.14%	0.012%
82	18.598	2636	2637	2639	rBV2	2382	1780	0.13%	0.011%
83	18.868	2679	2683	2689	rVB4	7234	9730	0.70%	0.060%
84	19.150	2728	2731	2736	rVB	12168	16607	1.20%	0.102%
85	19.239	2744	2746	2747	rBV2	2311	1599	0.12%	0.010%
86	19.403	2772	2774	2777	rBV	8028	8969	0.65%	0.055%
87	19.450	2780	2782	2786	rVB4	3919	4016	0.29%	0.025%
88	19.521	2788	2794	2800	rBV	1006913	1383532	100.00%	8.492%
89	19.750	2831	2833	2835	rVB2	3460	2635	0.19%	0.016%
90	20.439	2946	2950	2956	rVB4	14041	22936	1.66%	0.141%
91	21.021	3046	3049	3057	rBV	52795	74964	5.42%	0.460%
92	21.315	3094	3099	3110	rBV	811376	1011636	73.12%	6.209%
93	23.427	3451	3458	3466	rBV	507823	956776	69.15%	5.873%
94	23.574	3476	3483	3493	rVB2	480015	918142	66.36%	5.635%


Sum of corrected areas: 16292360

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
Data File : BM003539.D
Acq On : 14 Dec 2015 14:06
Operator : UM/IZ
Sample : G4722-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C9

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

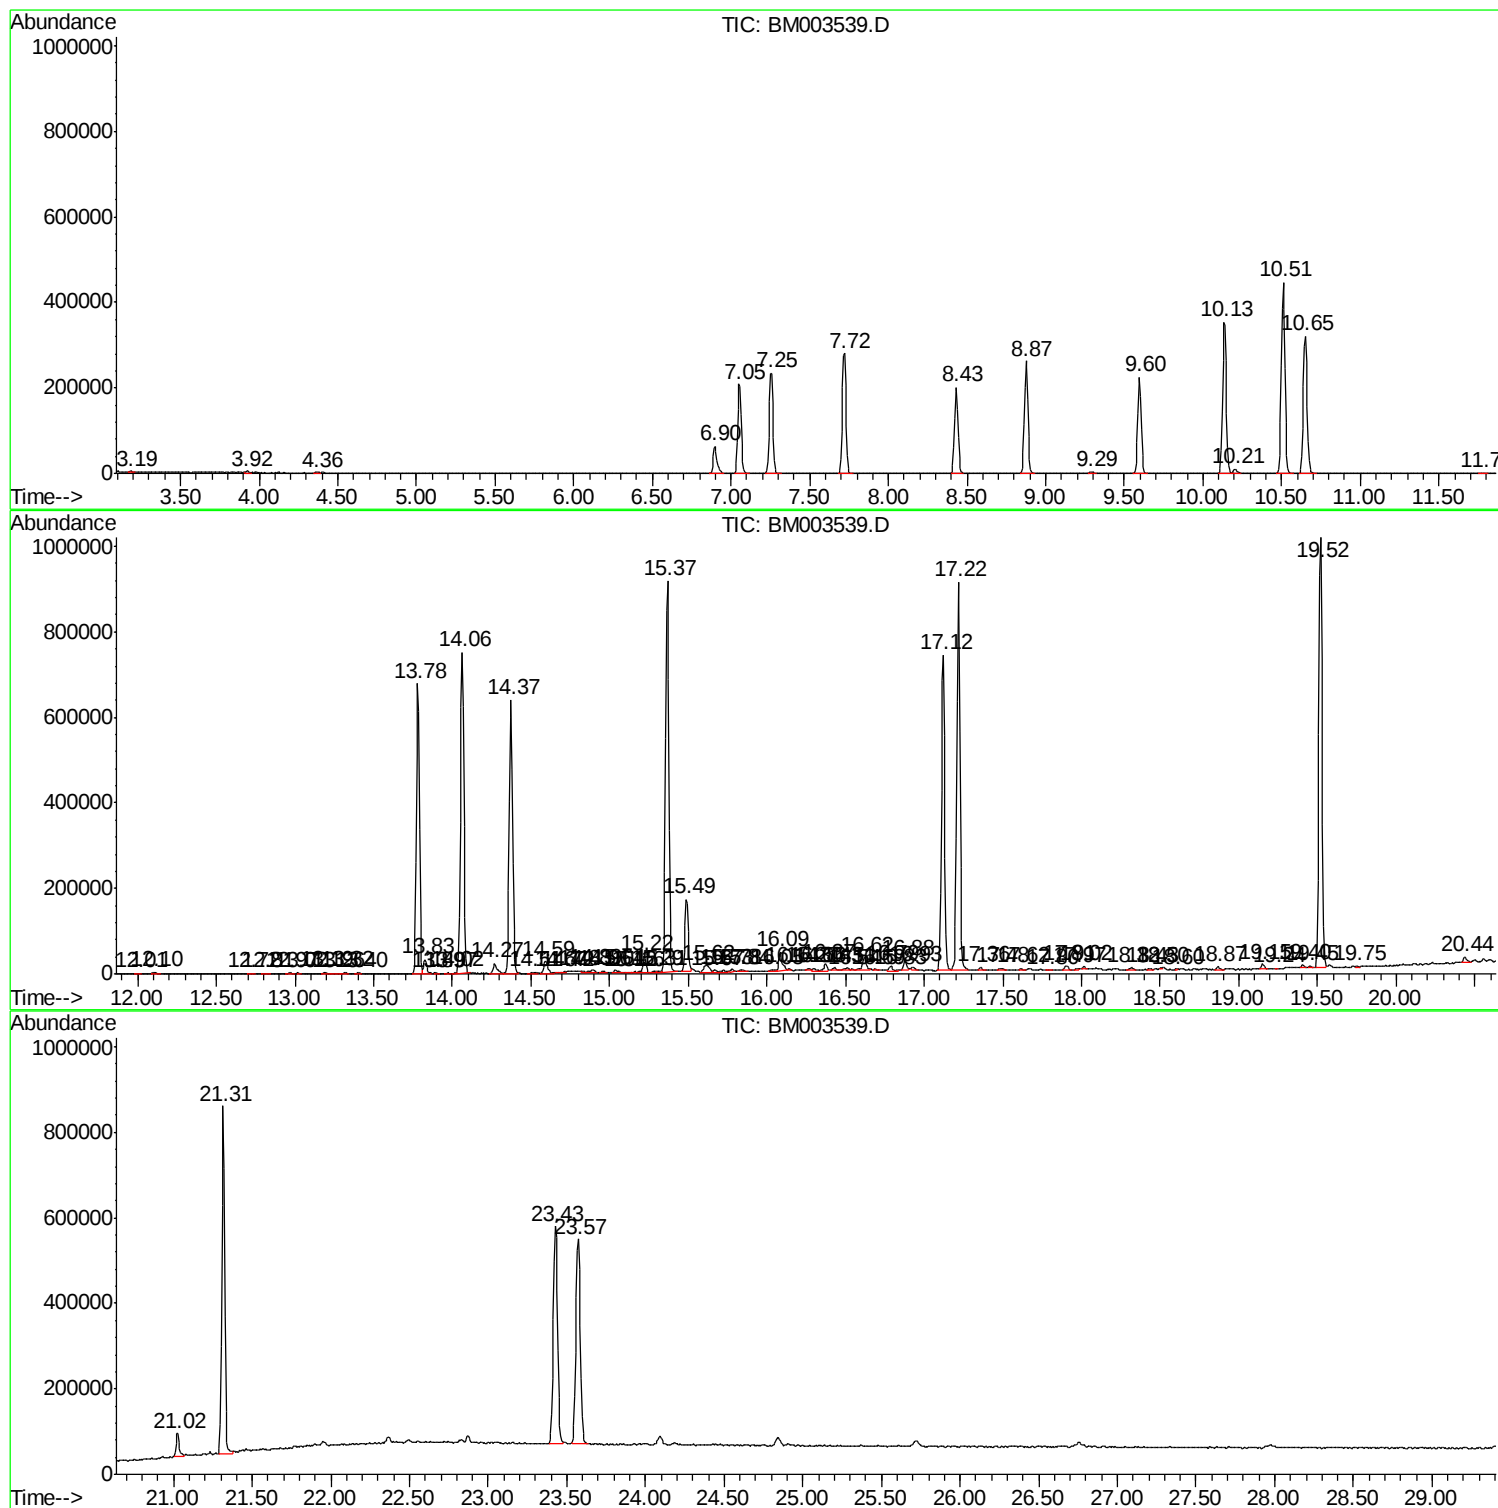

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003539.D
Acq On : 14 Dec 2015 14:06
Operator : UM/IZ
Sample : G4722-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C9

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003539.D
Acq On : 14 Dec 2015 14:06
Operator : UM/IZ
Sample : G4722-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C9

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc