

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
 Data File : BM003541.D
 Acq On : 14 Dec 2015 15:19
 Operator : UM/IZ
 Sample : G4722-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04D7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	21	rVB	4873	5685	0.33%	0.033%
2	4.287	200	204	208	rBV	2036	2108	0.12%	0.012%
3	6.899	639	648	655	rBB	79977	124812	7.26%	0.733%
4	7.051	667	674	684	rBB	281372	434426	25.27%	2.553%
5	7.251	702	708	717	rBB	310178	489046	28.45%	2.874%
6	7.722	781	788	796	rBB	246002	391670	22.78%	2.302%
7	7.793	797	800	804	rBB	1745	2405	0.14%	0.014%
8	8.093	848	851	857	rBB2	1097	1755	0.10%	0.010%
9	8.434	903	909	918	rBB	243885	378083	21.99%	2.222%
10	8.875	978	984	994	rBB	329688	537471	31.27%	3.158%
11	9.187	1032	1037	1042	rBB	20431	29427	1.71%	0.173%
12	9.598	1100	1107	1115	rBB	284973	453937	26.41%	2.667%
13	10.063	1182	1186	1191	rBB	6637	8896	0.52%	0.052%
14	10.139	1192	1199	1213	rBV	410546	692283	40.27%	4.068%
15	10.287	1221	1224	1226	rBV	2425	3089	0.18%	0.018%
16	10.310	1226	1228	1232	rVB	2532	2901	0.17%	0.017%
17	10.510	1255	1262	1268	rBV	345813	570464	33.19%	3.352%
18	10.563	1268	1271	1275	rVB	10433	14290	0.83%	0.084%
19	10.651	1283	1286	1290	rBV	1851	2801	0.16%	0.016%
20	11.616	1446	1450	1453	rBB2	2454	3271	0.19%	0.019%
21	11.863	1488	1492	1496	rBB	1678	2577	0.15%	0.015%
22	12.104	1529	1533	1537	rBB	5436	7959	0.46%	0.047%
23	12.345	1571	1574	1578	rBB2	4652	5849	0.34%	0.034%
24	12.398	1579	1583	1587	rBV	6178	8480	0.49%	0.050%
25	12.433	1587	1589	1593	rVB2	2271	2332	0.14%	0.014%
26	12.616	1615	1620	1626	rBV3	9125	13544	0.79%	0.080%
27	12.822	1653	1655	1659	rBV2	2492	2105	0.12%	0.012%
28	13.269	1726	1731	1734	rBB2	1923	2493	0.15%	0.015%
29	13.780	1812	1818	1829	rBV	725560	1002707	58.33%	5.892%
30	13.922	1838	1842	1845	rVB	2330	2936	0.17%	0.017%
31	14.063	1860	1866	1873	rBV	855539	1255733	73.05%	7.379%
32	14.127	1873	1877	1880	rVB2	5314	7522	0.44%	0.044%
33	14.292	1903	1905	1909	rVB	2165	1736	0.10%	0.010%
34	14.374	1912	1919	1926	rBV2	443783	687513	39.99%	4.040%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
 Data File : BM003541.D
 Acq On : 14 Dec 2015 15:19
 Operator : UM/IZ
 Sample : G4722-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04D7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	14.433	1926	1929	1935	rVB2	2672	3497	0.20%	0.021%
36	14.592	1951	1956	1965	rBV	42024	66894	3.89%	0.393%
37	14.733	1977	1980	1985	rVB2	1484	2002	0.12%	0.012%
38	15.033	2027	2031	2035	rBV2	1621	2003	0.12%	0.012%
39	15.116	2041	2045	2048	rBV	2239	3059	0.18%	0.018%
40	15.369	2081	2088	2100	rBV	1046454	1523116	88.60%	8.950%
41	15.492	2103	2109	2116	rBV	232667	330532	19.23%	1.942%
42	15.604	2124	2128	2135	rVB4	11953	18710	1.09%	0.110%
43	15.880	2170	2175	2183	rVV	17286	25455	1.48%	0.150%
44	16.057	2200	2205	2210	rVB2	5114	9525	0.55%	0.056%
45	16.210	2228	2231	2233	rBV2	2325	2015	0.12%	0.012%
46	16.263	2236	2240	2241	rBV	2636	2361	0.14%	0.014%
47	16.392	2258	2262	2267	rVB	6616	10480	0.61%	0.062%
48	16.510	2281	2282	2284	rBV	2119	1796	0.10%	0.011%
49	16.880	2339	2345	2350	rBV	95642	126463	7.36%	0.743%
50	16.921	2350	2352	2357	rVB	10481	13584	0.79%	0.080%
51	16.986	2357	2363	2369	rBV	36552	49907	2.90%	0.293%
52	17.080	2375	2379	2380	rBV2	6437	7108	0.41%	0.042%
53	17.121	2380	2386	2393	rVV	510065	741881	43.16%	4.359%
54	17.221	2396	2403	2413	rVB2	1012486	1524641	88.69%	8.959%
55	17.463	2442	2444	2446	rBV3	2741	1916	0.11%	0.011%
56	17.733	2485	2490	2492	rBV4	3132	4904	0.29%	0.029%
57	17.792	2498	2500	2504	rVB2	2613	2939	0.17%	0.017%
58	17.986	2531	2533	2536	rVV3	1962	1819	0.11%	0.011%
59	18.098	2547	2552	2557	rBV3	3670	7327	0.43%	0.043%
60	18.345	2590	2594	2595	rBV3	2872	3450	0.20%	0.020%
61	18.392	2601	2602	2609	rVB5	3484	3213	0.19%	0.019%
62	18.474	2614	2616	2619	rBV3	2244	2839	0.17%	0.017%
63	18.504	2619	2621	2624	rVB2	4272	3567	0.21%	0.021%
64	18.768	2665	2666	2672	rVB5	3333	3582	0.21%	0.021%
65	18.933	2692	2694	2698	rBV5	3883	3939	0.23%	0.023%
66	18.986	2701	2703	2704	rVV2	4315	2736	0.16%	0.016%
67	19.027	2708	2710	2713	rVB3	2148	2143	0.12%	0.013%
68	19.151	2726	2731	2740	rBV	15825	28477	1.66%	0.167%
69	19.233	2741	2745	2752	rVV	54465	72202	4.20%	0.424%
70	19.404	2771	2774	2779	rBV	11731	19456	1.13%	0.114%
71	19.451	2779	2782	2787	rVB4	13379	17157	1.00%	0.101%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
Data File : BM003541.D
Acq On : 14 Dec 2015 15:19
Operator : UM/IZ
Sample : G4722-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04D7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION

72	19.521	2788	2794	2799	rBV	1239363	1719034	100.00%	10.101%
73	19.568	2799	2802	2807	rVB	78417	104599	6.08%	0.615%
74	19.651	2813	2816	2822	rVB5	8198	10113	0.59%	0.059%
75	19.933	2862	2864	2868	rVB4	7363	6374	0.37%	0.037%
76	21.315	3094	3099	3106	rBV	690199	872824	50.77%	5.129%
77	23.433	3451	3459	3472	rVB	855160	1643939	95.63%	9.660%
78	23.574	3476	3483	3494	rVB	461855	861972	50.14%	5.065%


Sum of corrected areas: 17017856

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
Data File : BM003541.D
Acq On : 14 Dec 2015 15:19
Operator : UM/IZ
Sample : G4722-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04D7

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

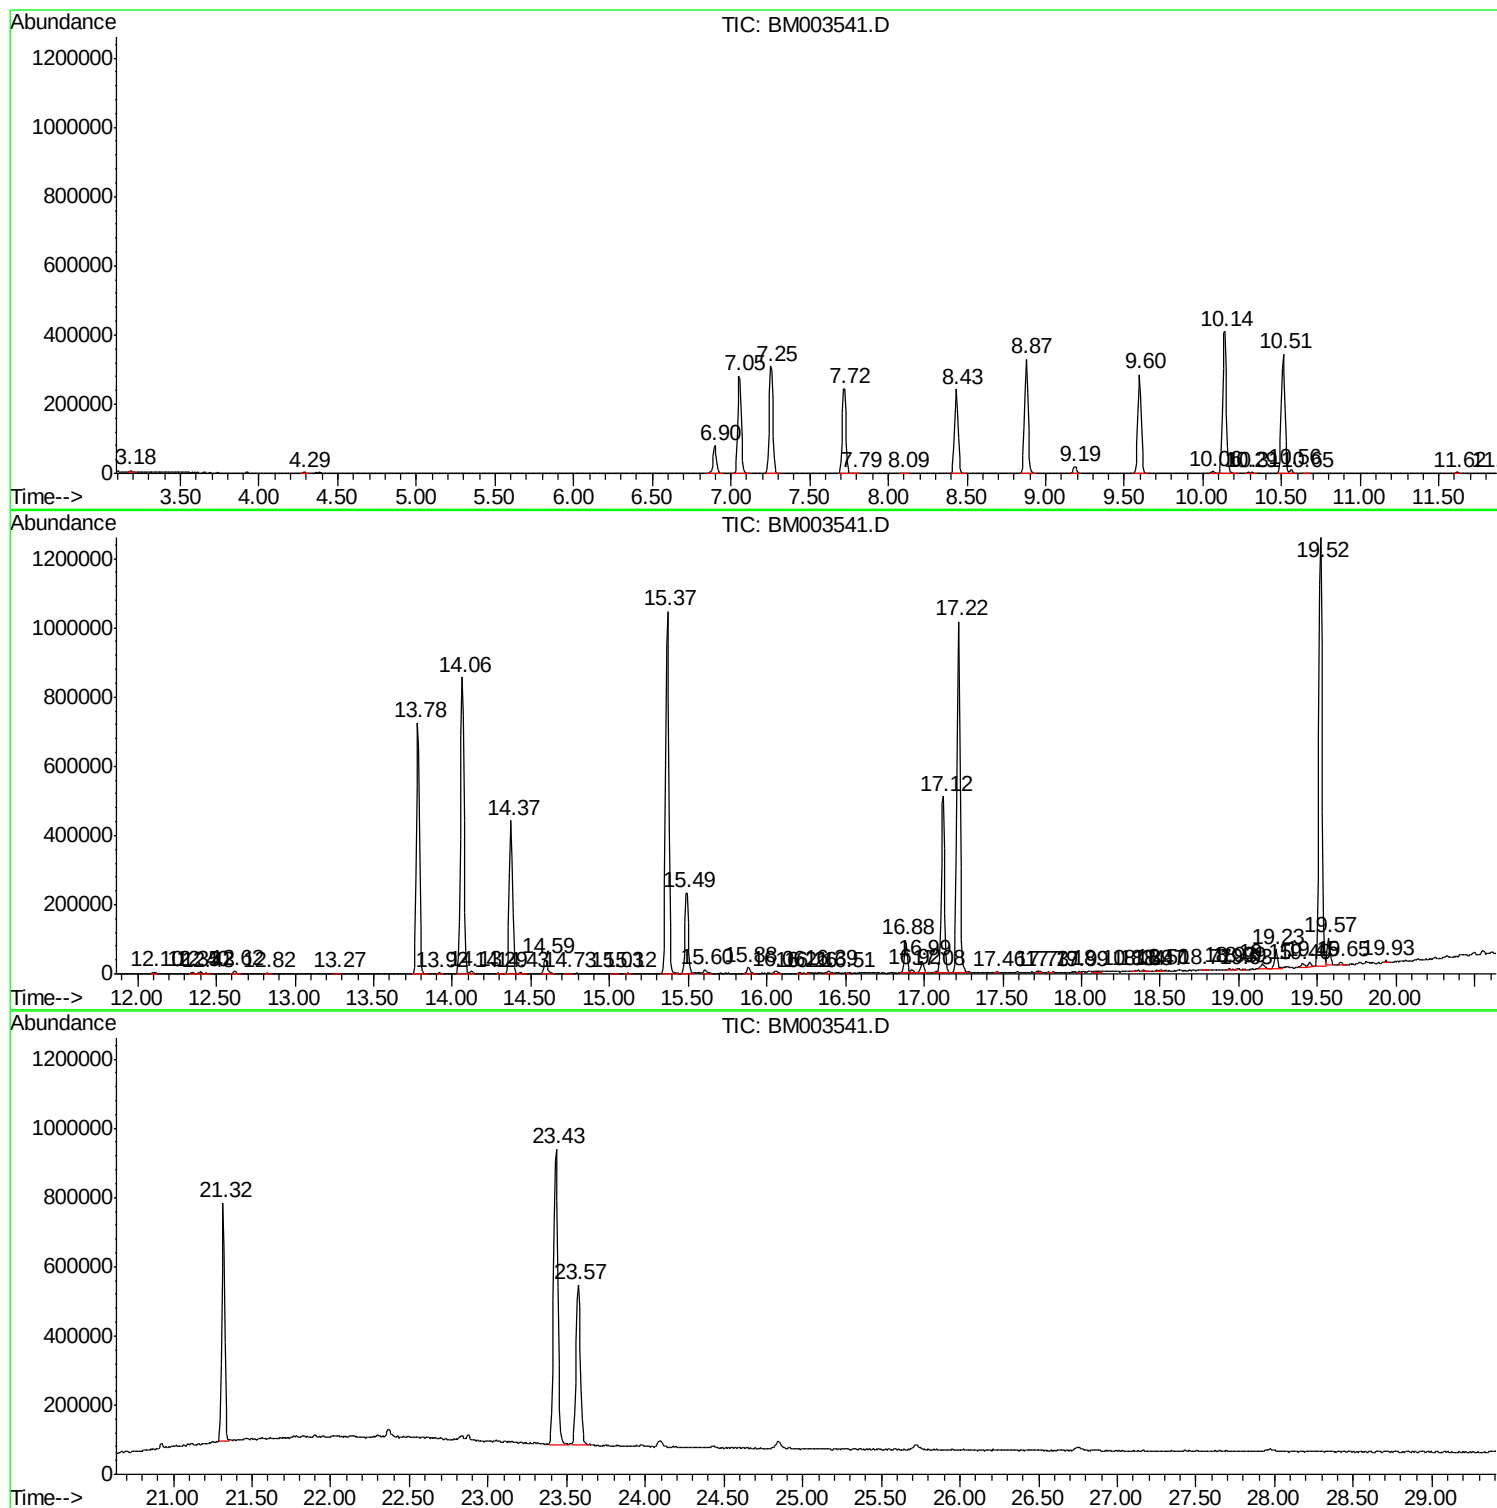

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003541.D
Acq On : 14 Dec 2015 15:19
Operator : UM/IZ
Sample : G4722-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04D7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003541.D
Acq On : 14 Dec 2015 15:19
Operator : UM/IZ
Sample : G4722-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04D7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc