

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
 Data File : BM003543.D
 Acq On : 14 Dec 2015 17:21
 Operator : UM/IZ
 Sample : PB87248BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK48

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	11	16	28	rVB	21268	28336	1.44%	0.142%
2	3.740	107	111	114	rBV	3112	3842	0.19%	0.019%
3	6.899	641	648	661	rVB	381018	588934	29.84%	2.949%
4	7.052	668	674	682	rBV	297437	464491	23.54%	2.326%
5	7.252	702	708	717	rBB	396642	624836	31.66%	3.129%
6	7.716	781	787	795	rBB	246694	388826	19.70%	1.947%
7	8.434	902	909	921	rBB	502300	791408	40.10%	3.963%
8	8.881	978	985	993	rBV	355031	575102	29.14%	2.880%
9	9.598	1101	1107	1116	rBB	302982	478931	24.27%	2.399%
10	10.140	1192	1199	1211	rBV	471613	785717	39.81%	3.935%
11	10.510	1255	1262	1271	rBB	373202	608707	30.84%	3.048%
12	10.651	1279	1286	1298	rBV	480690	806366	40.86%	4.038%
13	12.104	1529	1533	1538	rBB	6196	8553	0.43%	0.043%
14	13.781	1812	1818	1829	rBV	797878	1125120	57.01%	5.635%
15	14.063	1859	1866	1887	rBV	951568	1387650	70.32%	6.949%
16	14.375	1912	1919	1927	rBB2	512043	779039	39.48%	3.901%
17	14.586	1950	1955	1976	rBV	245776	380955	19.30%	1.908%
18	15.369	2081	2088	2097	rBV	1199832	1680179	85.14%	8.414%
19	15.492	2104	2109	2118	rVB	197642	256270	12.99%	1.283%
20	15.610	2125	2129	2133	rBB	10555	12785	0.65%	0.064%
21	17.122	2380	2386	2393	rBV	591106	810735	41.08%	4.060%
22	17.221	2396	2403	2418	rVV	1187187	1688539	85.56%	8.456%
23	19.157	2728	2732	2738	rBV	10217	13573	0.69%	0.068%
24	19.410	2770	2775	2778	rBV	7700	9692	0.49%	0.049%
25	19.451	2779	2782	2788	rVB3	5037	4802	0.24%	0.024%
26	19.521	2788	2794	2801	rBV	1401496	1855045	94.00%	9.290%
27	20.339	2931	2933	2938	rBV4	1526	2300	0.12%	0.012%
28	20.504	2958	2961	2963	rBV2	5041	4331	0.22%	0.022%
29	21.315	3094	3099	3109	rBV	696933	911436	46.18%	4.565%
30	21.468	3122	3125	3128	rBV2	4538	5287	0.27%	0.026%
31	22.833	3355	3357	3361	rVB3	12483	12651	0.64%	0.063%
32	23.433	3451	3459	3471	rBV	1036713	1973474	100.00%	9.883%
33	23.580	3476	3484	3495	rVB2	459183	899885	45.60%	4.507%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
Data File : BM003543.D
Acq On : 14 Dec 2015 17:21
Operator : UM/IZ
Sample : PB87248BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK48

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION


Sum of corrected areas: 19967797

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
Data File : BM003543.D
Acq On : 14 Dec 2015 17:21
Operator : UM/IZ
Sample : PB87248BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK48

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

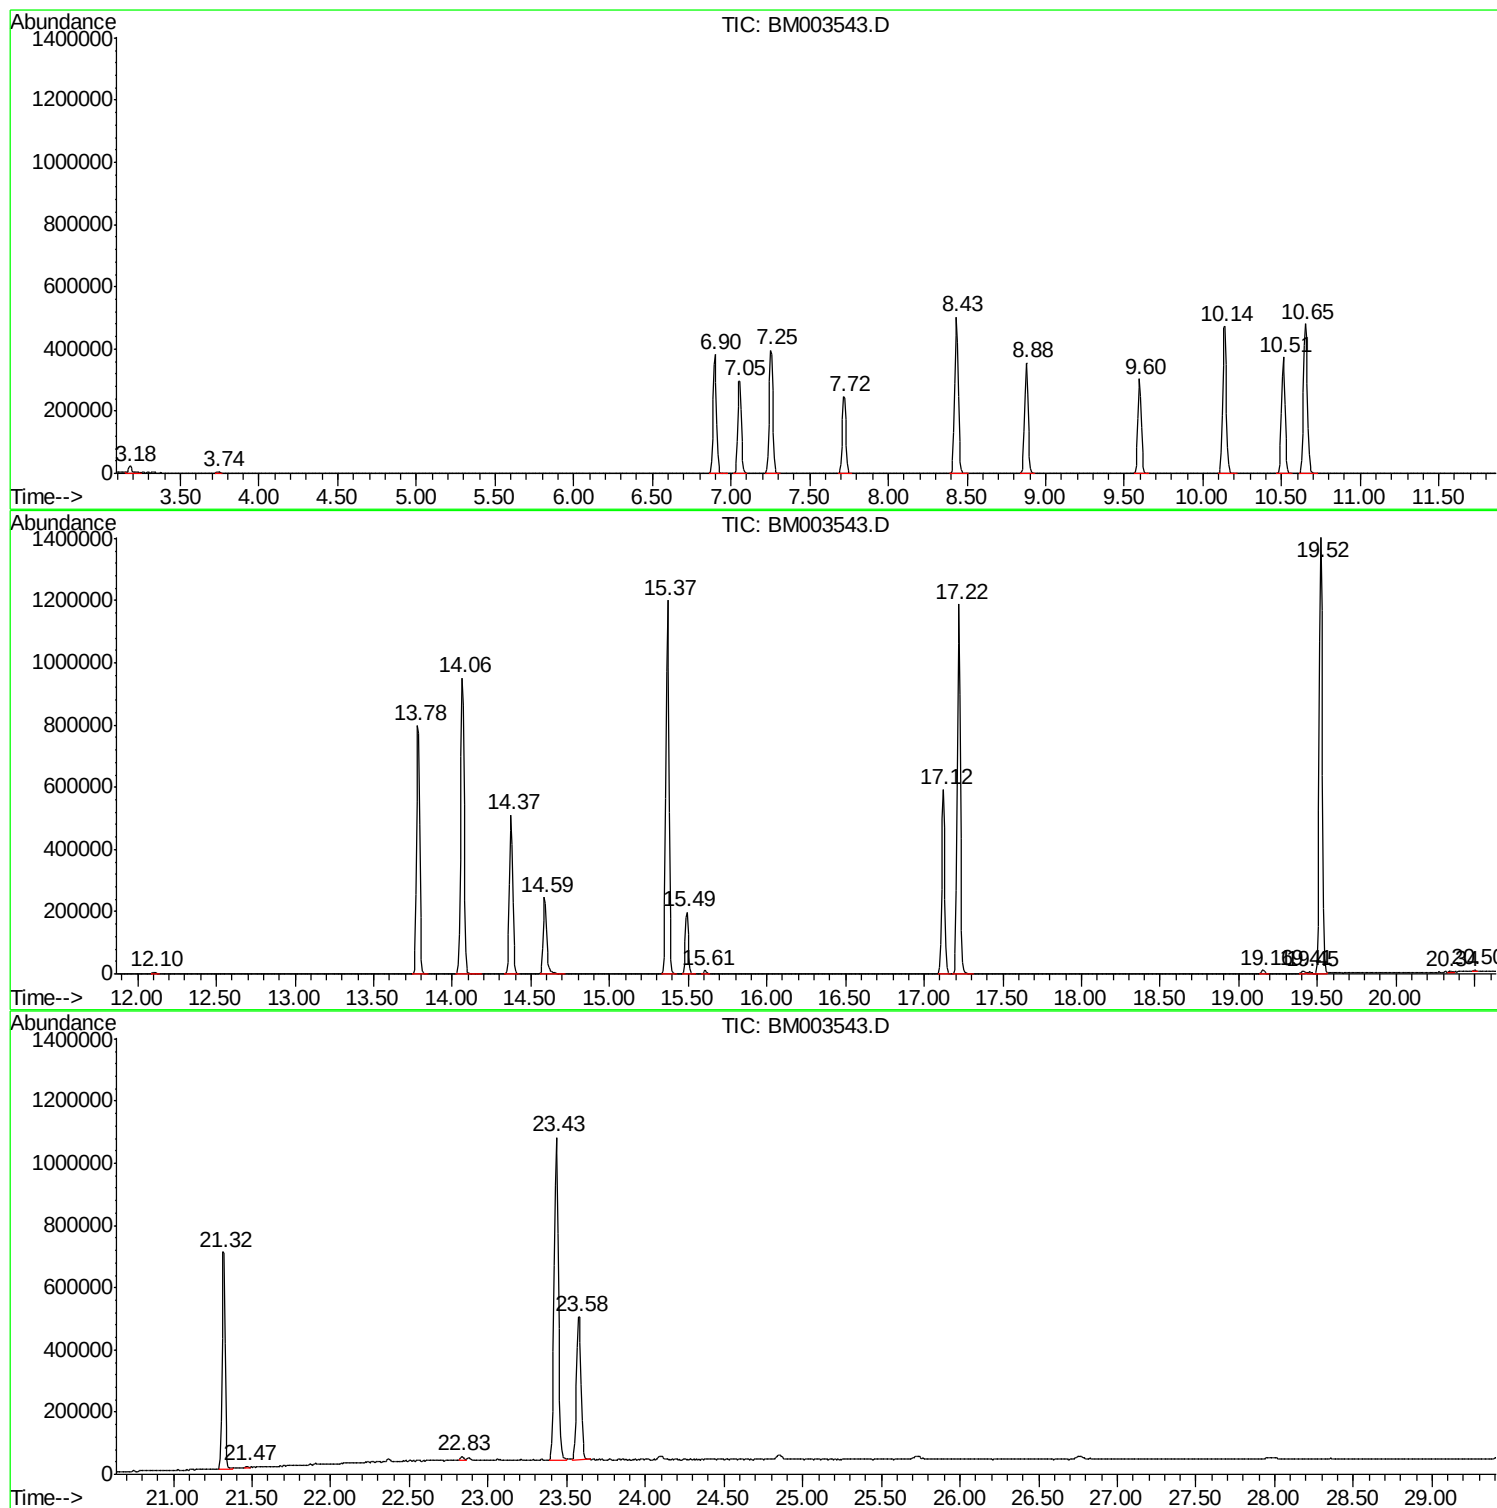

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003543.D
Acq On : 14 Dec 2015 17:21
Operator : UM/IZ
Sample : PB87248BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK48

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003543.D
Acq On : 14 Dec 2015 17:21
Operator : UM/IZ
Sample : PB87248BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK48

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc