

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
 Data File : BM003544.D
 Acq On : 14 Dec 2015 17:57
 Operator : UM/IZ
 Sample : G4722-19
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04C7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	13	17	20	rVB	4323	5137	0.33%	0.031%
2	3.475	62	66	73	rVB3	1572	2741	0.18%	0.017%
3	4.375	215	219	225	rVB2	1352	2805	0.18%	0.017%
4	6.898	642	648	655	rVB	80640	124718	8.08%	0.761%
5	7.051	668	674	685	rBV	288809	447204	28.97%	2.730%
6	7.251	702	708	718	rBB	315294	505631	32.75%	3.086%
7	7.716	781	787	794	rBB	269280	427263	27.68%	2.608%
8	8.434	903	909	919	rBB	245239	388739	25.18%	2.373%
9	8.781	964	968	970	rBB	1317	1761	0.11%	0.011%
10	8.875	978	984	994	rBB	343015	551198	35.70%	3.364%
11	9.598	1100	1107	1114	rBB	285125	461716	29.91%	2.818%
12	10.134	1192	1198	1213	rBV	422286	702386	45.50%	4.287%
13	10.510	1255	1262	1269	rBV	385767	634381	41.09%	3.872%
14	10.657	1283	1287	1291	rBB	1376	1876	0.12%	0.011%
15	11.763	1469	1475	1481	rBB2	5244	8169	0.53%	0.050%
16	11.963	1505	1509	1513	rBB2	1437	2073	0.13%	0.013%
17	12.104	1529	1533	1537	rBB	5626	8180	0.53%	0.050%
18	12.175	1541	1545	1550	rBB2	5691	8131	0.53%	0.050%
19	12.245	1550	1557	1561	rBB	1718	2945	0.19%	0.018%
20	12.422	1584	1587	1592	rBB	2973	4140	0.27%	0.025%
21	12.739	1635	1641	1645	rBV3	3764	7545	0.49%	0.046%
22	12.775	1645	1647	1650	rVV3	2144	2770	0.18%	0.017%
23	12.804	1650	1652	1656	rVV2	2031	2759	0.18%	0.017%
24	12.886	1660	1666	1670	rBV3	4666	9543	0.62%	0.058%
25	12.939	1671	1675	1677	rVV3	2041	3725	0.24%	0.023%
26	12.974	1677	1681	1685	rVV	3478	4855	0.31%	0.030%
27	13.027	1685	1690	1698	rVB4	3663	8244	0.53%	0.050%
28	13.092	1698	1701	1703	rBV3	1475	1981	0.13%	0.012%
29	13.139	1703	1709	1710	rVB4	1139	1869	0.12%	0.011%
30	13.269	1727	1731	1734	rVV3	3626	5021	0.33%	0.031%
31	13.322	1738	1740	1744	rVV2	1804	2493	0.16%	0.015%
32	13.374	1744	1749	1756	rVV3	3222	5894	0.38%	0.036%
33	13.445	1756	1761	1766	rVB3	1697	3894	0.25%	0.024%
34	13.551	1775	1779	1782	rBV2	1739	3536	0.23%	0.022%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
 Data File : BM003544.D
 Acq On : 14 Dec 2015 17:57
 Operator : UM/IZ
 Sample : G4722-19
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04C7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	13.586	1782	1785	1787	rBV2	1480	2003	0.13%	0.012%
36	13.780	1808	1818	1827	rVB	739152	1013526	65.65%	6.186%
37	13.869	1831	1833	1836	rVB3	1842	2042	0.13%	0.012%
38	13.921	1838	1842	1846	rVB6	1696	2746	0.18%	0.017%
39	13.974	1846	1851	1855	rBV5	1869	3478	0.23%	0.021%
40	14.063	1859	1866	1877	rBV	870490	1269163	82.21%	7.747%
41	14.180	1884	1886	1889	rBV2	1380	1551	0.10%	0.009%
42	14.269	1897	1901	1902	rBV4	1558	2318	0.15%	0.014%
43	14.292	1902	1905	1909	rVV2	6791	10945	0.71%	0.067%
44	14.374	1909	1919	1926	rVV2	493774	769872	49.87%	4.699%
45	14.433	1926	1929	1932	rVV2	3070	3791	0.25%	0.023%
46	14.592	1951	1956	1965	rBV	39103	71159	4.61%	0.434%
47	14.863	2000	2002	2005	rVB3	3468	3221	0.21%	0.020%
48	14.916	2006	2011	2016	rVB5	6949	12491	0.81%	0.076%
49	15.033	2026	2031	2034	rBV	14358	19073	1.24%	0.116%
50	15.368	2081	2088	2097	rBV	1026869	1495704	96.89%	9.130%
51	15.492	2103	2109	2116	rBV	221686	320350	20.75%	1.955%
52	15.604	2124	2128	2132	rBV	12475	17158	1.11%	0.105%
53	15.880	2173	2175	2176	rBV2	3003	2465	0.16%	0.015%
54	16.021	2198	2199	2202	rBV3	4283	4431	0.29%	0.027%
55	16.115	2212	2215	2218	rVB2	6700	8040	0.52%	0.049%
56	16.204	2226	2230	2236	rBV	14741	26467	1.71%	0.162%
57	16.268	2237	2241	2246	rVV5	14624	25484	1.65%	0.156%
58	16.327	2246	2251	2255	rVV4	16668	24437	1.58%	0.149%
59	16.374	2255	2259	2263	rVB4	8880	13300	0.86%	0.081%
60	16.451	2266	2272	2274	rBV2	6511	13010	0.84%	0.079%
61	16.474	2274	2276	2279	rVB4	4693	4164	0.27%	0.025%
62	16.527	2281	2285	2292	rVB3	15982	32260	2.09%	0.197%
63	16.592	2292	2296	2300	rBV	19342	28658	1.86%	0.175%
64	16.674	2306	2310	2313	rVB2	8378	11905	0.77%	0.073%
65	17.121	2379	2386	2396	rBV2	537590	787842	51.03%	4.809%
66	17.215	2396	2402	2415	rVB2	979694	1433022	92.83%	8.747%
67	18.015	2536	2538	2543	rVB6	8107	9286	0.60%	0.057%
68	18.521	2621	2624	2632	rVB	29344	41897	2.71%	0.256%
69	19.521	2788	2794	2807	rBV	1069784	1543779	100.00%	9.423%
70	21.315	3094	3099	3106	rBV	666400	836723	54.20%	5.107%
71	23.427	3451	3458	3466	rBV	687143	1305627	84.57%	7.969%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
Data File : BM003544.D
Acq On : 14 Dec 2015 17:57
Operator : UM/IZ
Sample : G4722-19
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION

72	23.574	3476	3483	3494	rVB	441622	854335	55.34%	5.215%
----	--------	------	------	------	-----	--------	--------	--------	--------


Sum of corrected areas: 16383046

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
Data File : BM003544.D
Acq On : 14 Dec 2015 17:57
Operator : UM/IZ
Sample : G4722-19
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C7

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

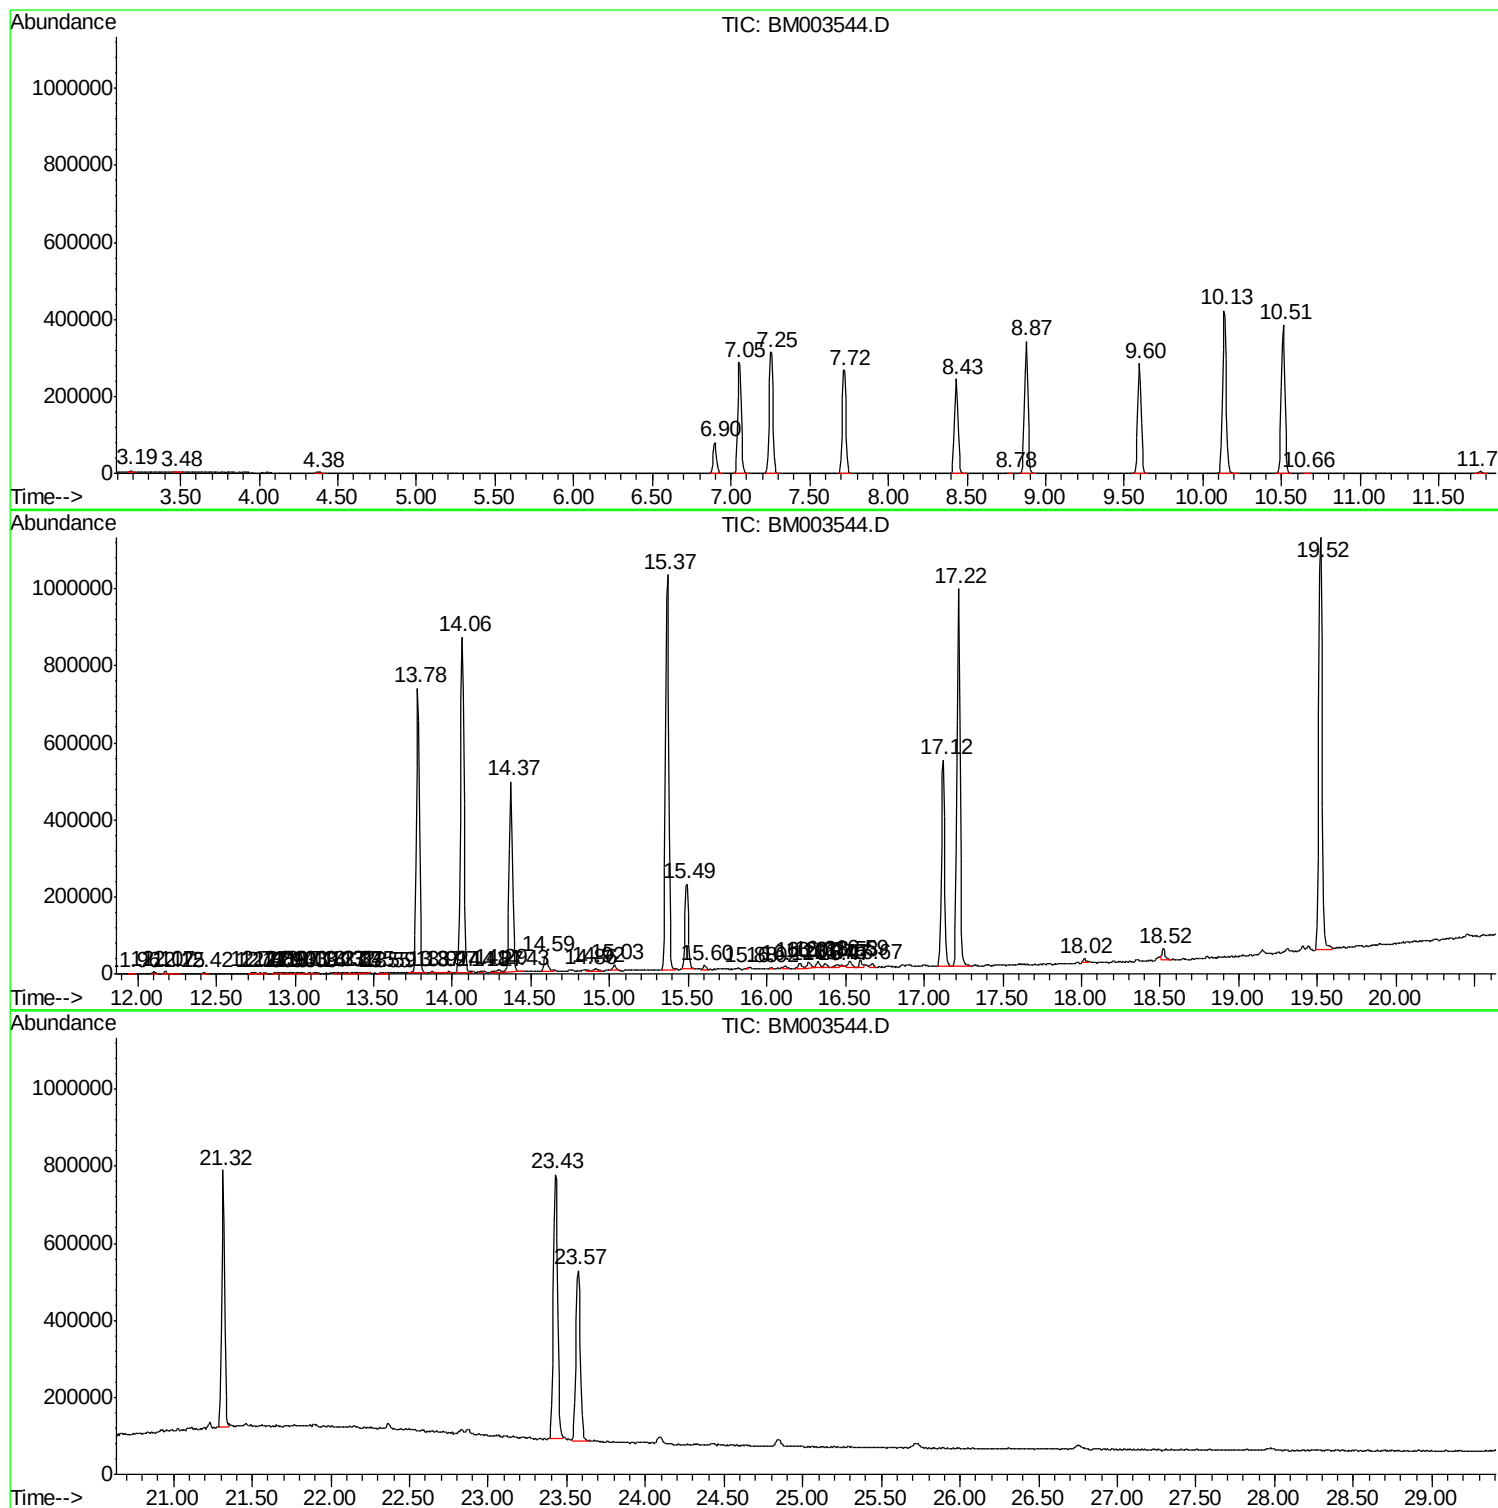

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003544.D
Acq On : 14 Dec 2015 17:57
Operator : UM/IZ
Sample : G4722-19
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003544.D
Acq On : 14 Dec 2015 17:57
Operator : UM/IZ
Sample : G4722-19
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc