

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
 Data File : BM003546.D
 Acq On : 14 Dec 2015 19:10
 Operator : UM/IZ
 Sample : G4722-22
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04F4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	14	17	19	rVB2	1513	1706	0.18%	0.015%
2	5.234	361	365	370	rBB	3382	4759	0.49%	0.043%
3	6.898	643	648	657	rVB2	35683	57445	5.92%	0.514%
4	7.051	669	674	683	rBB	125744	190555	19.65%	1.704%
5	7.251	703	708	716	rBB	136662	210908	21.75%	1.886%
6	7.722	781	788	794	rBB	263612	419725	43.29%	3.754%
7	7.787	795	799	802	rBB	2629	2995	0.31%	0.027%
8	8.092	847	851	855	rBB	4164	5561	0.57%	0.050%
9	8.434	903	909	917	rBB	110798	170667	17.60%	1.526%
10	8.875	978	984	992	rBB	147646	238610	24.61%	2.134%
11	9.292	1051	1055	1058	rBB	1779	2193	0.23%	0.020%
12	9.598	1101	1107	1113	rBB	122737	191982	19.80%	1.717%
13	10.139	1192	1199	1211	rBB	198479	330008	34.04%	2.952%
14	10.510	1255	1262	1268	rBV	416932	681838	70.32%	6.098%
15	10.563	1268	1271	1276	rVB	24678	34064	3.51%	0.305%
16	10.651	1279	1286	1300	rBV	186814	306947	31.66%	2.745%
17	12.104	1530	1533	1537	rBB	2319	2983	0.31%	0.027%
18	12.180	1542	1546	1550	rBB	3525	5176	0.53%	0.046%
19	12.398	1580	1583	1587	rBB	4472	6370	0.66%	0.057%
20	13.192	1715	1718	1721	rBB	2584	2675	0.28%	0.024%
21	13.780	1812	1818	1823	rBV	399592	526655	54.32%	4.710%
22	13.827	1823	1826	1834	rVB	30289	39325	4.06%	0.352%
23	14.063	1860	1866	1884	rBV	414604	591422	61.00%	5.290%
24	14.269	1897	1901	1905	rBB	15327	18437	1.90%	0.165%
25	14.374	1912	1919	1927	rBV2	580961	902519	93.08%	8.072%
26	14.433	1927	1929	1932	rVB	1937	2219	0.23%	0.020%
27	14.592	1952	1956	1965	rBB2	10811	17388	1.79%	0.156%
28	14.716	1974	1977	1979	rBV	2605	3551	0.37%	0.032%
29	14.733	1979	1980	1984	rVV3	2611	3214	0.33%	0.029%
30	14.774	1984	1987	1992	rVB	2323	3154	0.33%	0.028%
31	14.833	1993	1997	1999	rBB	2607	2596	0.27%	0.023%
32	14.892	2002	2007	2010	rBB	3720	5375	0.55%	0.048%
33	14.957	2015	2018	2021	rBB	2690	2910	0.30%	0.026%
34	15.116	2041	2045	2050	rBB2	2910	3780	0.39%	0.034%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
 Data File : BM003546.D
 Acq On : 14 Dec 2015 19:10
 Operator : UM/IZ
 Sample : G4722-22
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04F4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	15.174	2051	2055	2056	rBV2	1887	1975	0.20%	0.018%
36	15.221	2058	2063	2069	rVB	24162	30885	3.19%	0.276%
37	15.280	2069	2073	2077	rBV	2169	3496	0.36%	0.031%
38	15.316	2077	2079	2082	rVB	1393	1525	0.16%	0.014%
39	15.368	2082	2088	2095	rBV	517864	758591	78.24%	6.785%
40	15.416	2095	2096	2099	rVB3	2056	1662	0.17%	0.015%
41	15.492	2104	2109	2115	rVB	71142	98182	10.13%	0.878%
42	15.610	2121	2129	2131	rBV2	8098	12782	1.32%	0.114%
43	15.668	2137	2139	2142	rVB	2379	2060	0.21%	0.018%
44	15.721	2144	2148	2152	rBV3	3196	3964	0.41%	0.035%
45	15.786	2154	2159	2165	rBV3	5727	9504	0.98%	0.085%
46	15.845	2165	2169	2173	rVB3	4183	5929	0.61%	0.053%
47	16.027	2196	2200	2201	rBV2	2807	3741	0.39%	0.033%
48	16.086	2205	2210	2218	rBV	25706	41125	4.24%	0.368%
49	16.262	2237	2240	2243	rBV3	2854	3416	0.35%	0.031%
50	16.298	2243	2246	2249	rVB3	3281	3692	0.38%	0.033%
51	16.351	2251	2255	2256	rBV2	1587	1837	0.19%	0.016%
52	16.427	2264	2268	2271	rBV2	3074	4673	0.48%	0.042%
53	16.504	2276	2281	2285	rVV3	3399	7355	0.76%	0.066%
54	16.545	2285	2288	2290	rVV	1949	2440	0.25%	0.022%
55	16.574	2290	2293	2294	rVV3	2455	2114	0.22%	0.019%
56	16.592	2294	2296	2301	rVV3	2667	3657	0.38%	0.033%
57	16.657	2301	2307	2310	rVV3	2686	3823	0.39%	0.034%
58	16.692	2310	2313	2316	rVB2	1734	1677	0.17%	0.015%
59	16.786	2327	2329	2333	rVB	1740	1716	0.18%	0.015%
60	16.874	2339	2344	2348	rBV2	15056	20903	2.16%	0.187%
61	16.904	2348	2349	2351	rVV	3247	3265	0.34%	0.029%
62	16.951	2351	2357	2364	rVB5	6757	14719	1.52%	0.132%
63	17.027	2366	2370	2375	rVB2	1863	3768	0.39%	0.034%
64	17.121	2379	2386	2392	rBV	680116	965098	99.54%	8.632%
65	17.215	2395	2402	2415	rVB2	503084	741167	76.44%	6.629%
66	17.409	2431	2435	2437	rBV	1930	3179	0.33%	0.028%
67	17.474	2443	2446	2448	rBV2	1876	2140	0.22%	0.019%
68	17.504	2448	2451	2454	rVB2	1303	1674	0.17%	0.015%
69	17.545	2454	2458	2459	rVB2	1371	1773	0.18%	0.016%
70	17.580	2461	2464	2466	rVV2	1702	1794	0.19%	0.016%
71	17.615	2466	2470	2474	rVV	4570	6556	0.68%	0.059%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
 Data File : BM003546.D
 Acq On : 14 Dec 2015 19:10
 Operator : UM/IZ
 Sample : G4722-22
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04F4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

72	17.733	2488	2490	2493	rVV2	1265	1503	0.16%	0.013%
73	17.851	2504	2510	2513	rVB2	1396	1898	0.20%	0.017%
74	17.904	2513	2519	2527	rBV2	5404	9974	1.03%	0.089%
75	17.974	2527	2531	2532	rBV4	2150	2542	0.26%	0.023%
76	18.015	2533	2538	2541	rVB3	2966	4908	0.51%	0.044%
77	18.045	2541	2543	2544	rBV	1857	1511	0.16%	0.014%
78	18.092	2547	2551	2556	rVV2	1612	2732	0.28%	0.024%
79	18.315	2585	2589	2592	rBV3	3574	5306	0.55%	0.047%
80	18.527	2620	2625	2628	rVB2	3465	4876	0.50%	0.044%
81	18.780	2663	2668	2672	rVV2	1919	2740	0.28%	0.025%
82	18.868	2679	2683	2686	rVB	3064	4065	0.42%	0.036%
83	19.156	2727	2732	2735	rBV	3523	4797	0.49%	0.043%
84	19.409	2771	2775	2777	rBV	4118	5547	0.57%	0.050%
85	19.451	2777	2782	2785	rVV	14072	16326	1.68%	0.146%
86	19.521	2788	2794	2799	rVV	555304	775119	79.94%	6.933%
87	19.568	2799	2802	2807	rVV4	5563	7447	0.77%	0.067%
88	19.898	2854	2858	2862	rBV3	1423	2323	0.24%	0.021%
89	20.039	2880	2882	2885	rBV4	1498	1838	0.19%	0.016%
90	20.498	2957	2960	2965	rBV	13242	13712	1.41%	0.123%
91	20.556	2968	2970	2975	rVV3	3767	4537	0.47%	0.041%
92	20.603	2975	2978	2981	rVV5	2260	2874	0.30%	0.026%
93	21.027	3046	3050	3056	rBV3	30280	44975	4.64%	0.402%
94	21.227	3081	3084	3087	rBV	9816	10176	1.05%	0.091%
95	21.315	3093	3099	3107	rBV	760207	969600	100.00%	8.672%
96	22.362	3274	3277	3282	rVB2	16388	20822	2.15%	0.186%
97	22.874	3360	3364	3370	rVB3	17368	25961	2.68%	0.232%
98	23.427	3451	3458	3467	rBV	268124	524497	54.09%	4.691%
99	23.574	3475	3483	3492	rVB2	468011	905852	93.43%	8.102%
100	24.091	3568	3571	3577	rVB3	20400	34868	3.60%	0.312%


Sum of corrected areas: 11180895

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121415\
Data File : BM003546.D
Acq On : 14 Dec 2015 19:10
Operator : UM/IZ
Sample : G4722-22
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
C04F4

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

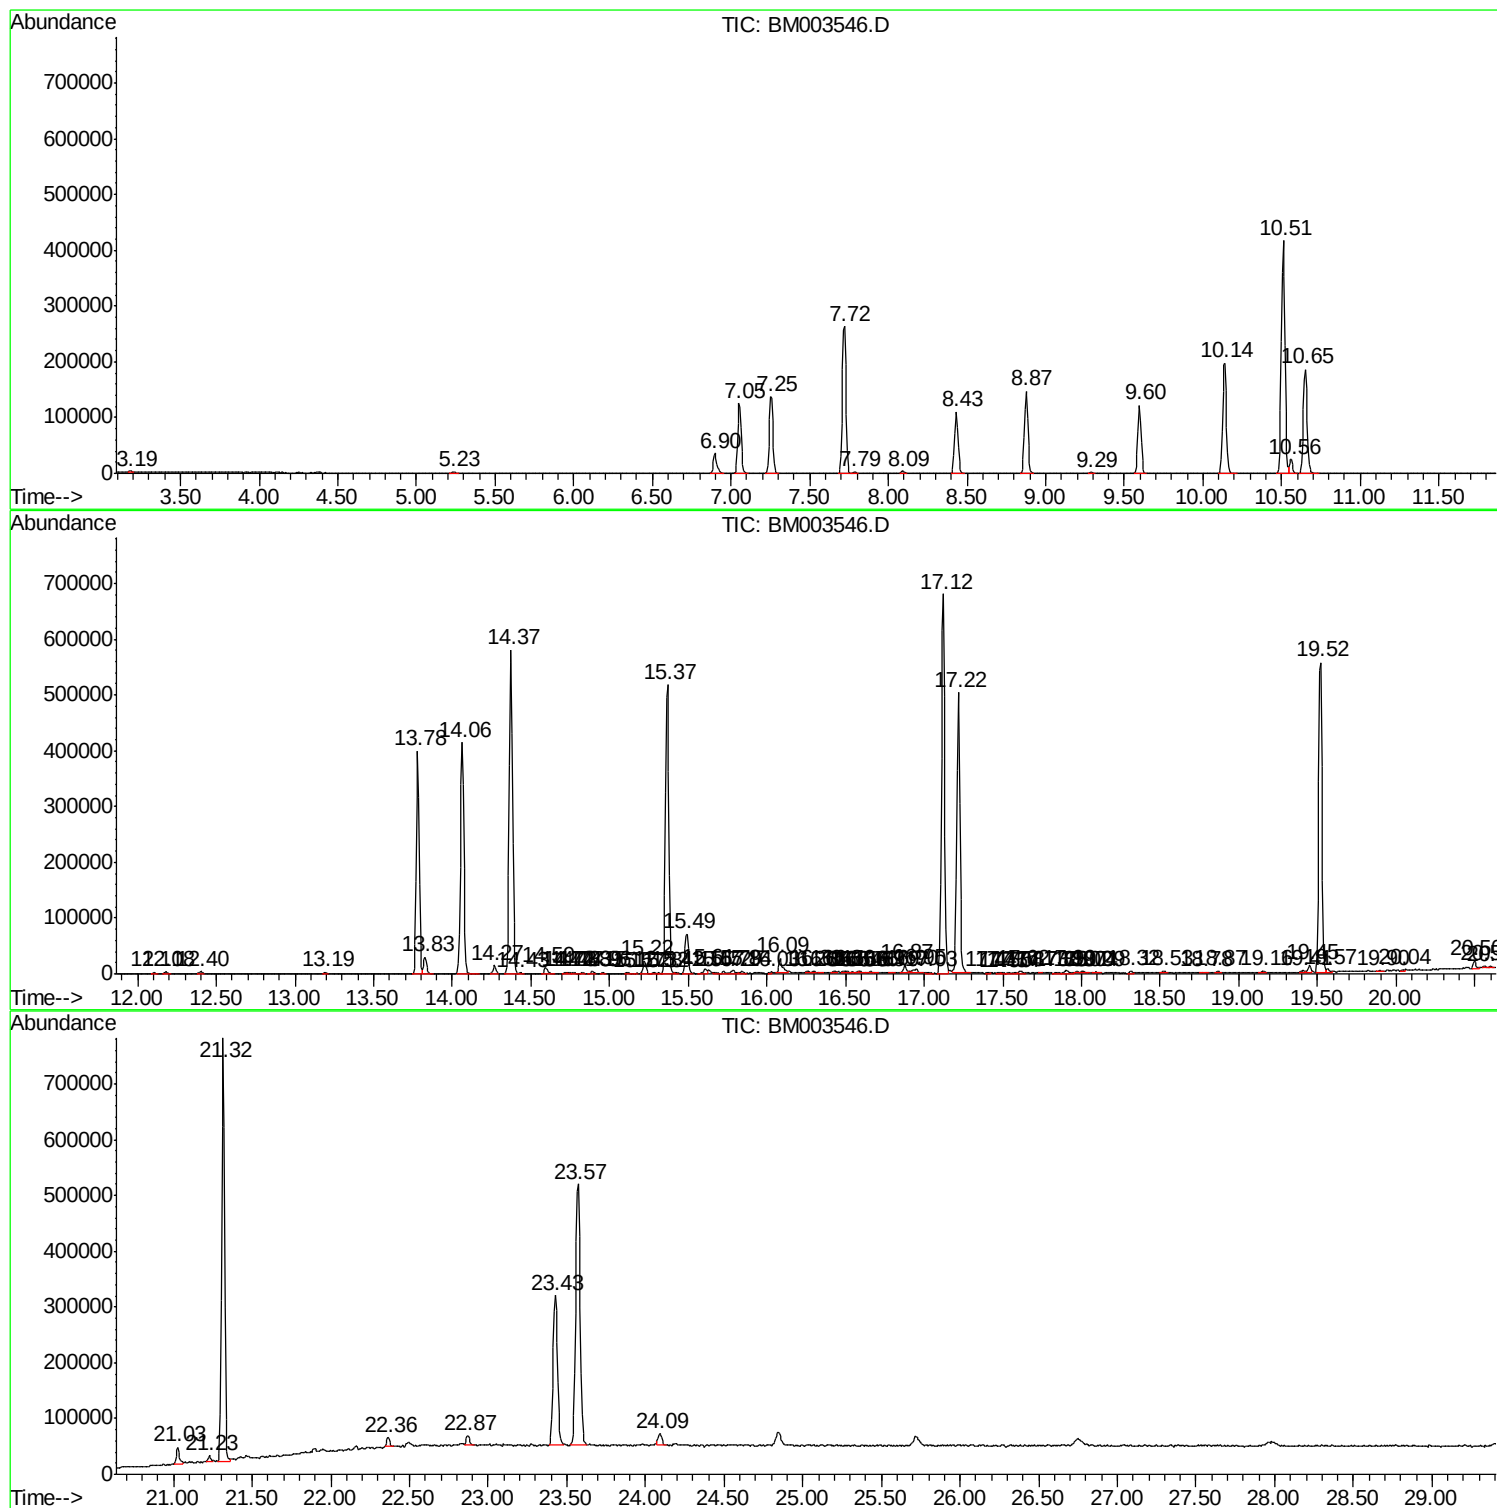

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003546.D
Acq On : 14 Dec 2015 19:10
Operator : UM/IZ
Sample : G4722-22
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04F4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121415\
Data File : BM003546.D
Acq On : 14 Dec 2015 19:10
Operator : UM/IZ
Sample : G4722-22
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04F4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc