


Data Path : Z:\HPCHEM1\BNA M\Data\BM121415\
 Data File : BM003532.D
 Acq On : 14 Dec 2015 09:03
 Operator : UM/IZ
 Sample : DFTPP57
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP57

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION
 Last Update : Tue Dec 15 13:44:42 2015

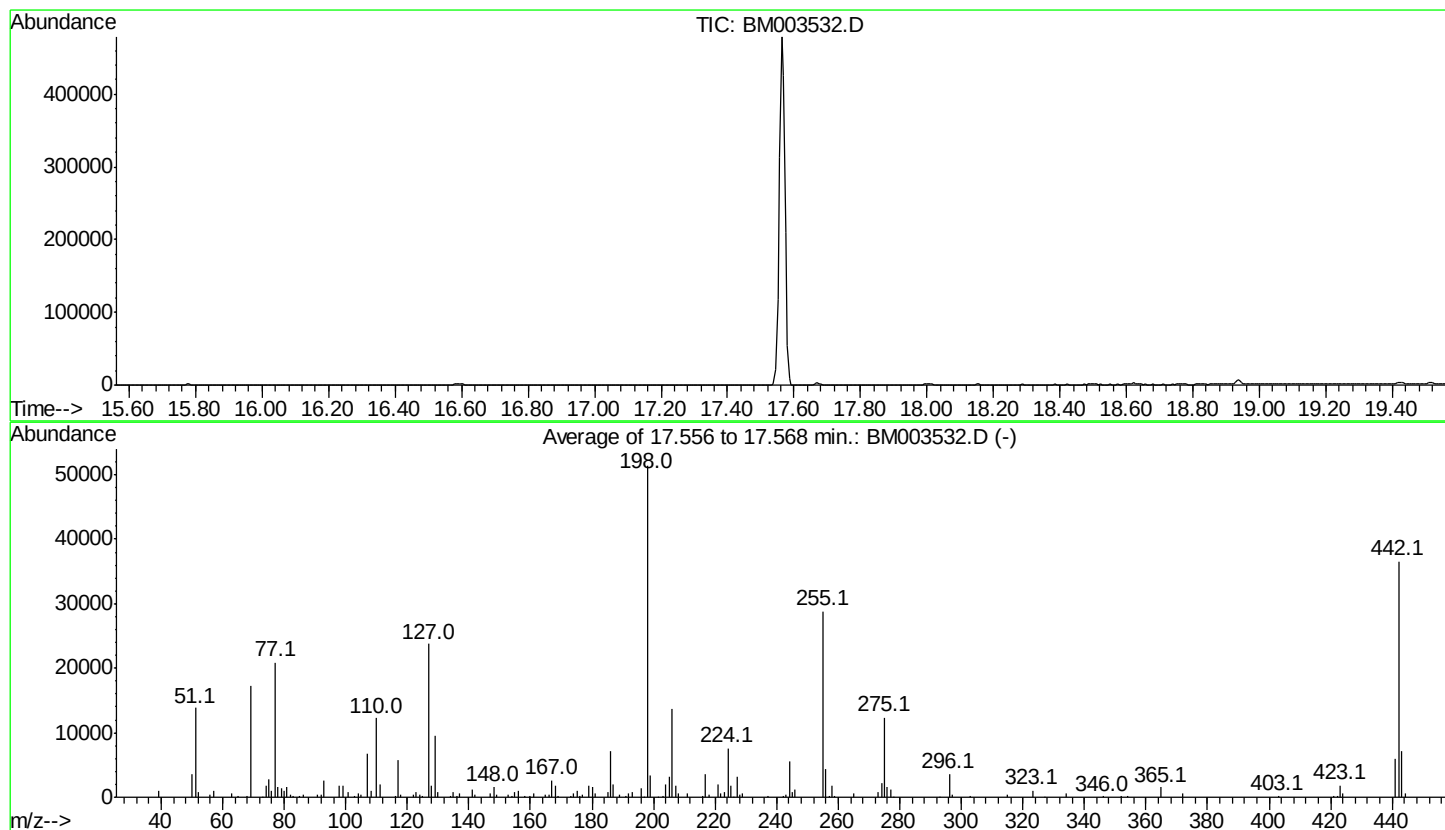

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	13885	PASS
68	69	0.00	2	0.7	123	PASS
69	198	0.00	100	33.5	17204	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.2	23749	PASS
197	198	0.00	2	0.2	101	PASS
198	198	100	100	100.0	51397	PASS
199	198	5	9	6.8	3476	PASS
275	198	10	60	24.0	12357	PASS
365	198	1	100	3.0	1527	PASS
441	443	0.01	100	81.4	5873	PASS
442	198	50	100	71.2	36589	PASS
443	442	15	24	19.7	7218	PASS

Scan 2455 (17.527 min): BM003532.D
DFTPP57

m/z	Abundance
73.00	333.0
207.10	445.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

m/z	Abundance
39.00	942.0
50.10	3109.0
51.10	12520.0
52.00	688.0
56.00	367.0
57.00	864.0
63.10	573.0
69.00	15811.0
73.00	302.0
74.00	1630.0
75.00	2585.0
76.00	769.0
77.10	18424.0
78.00	1342.0
79.00	1272.0
80.00	927.0
81.00	1389.0
82.00	333.0
86.00	333.0
90.90	355.0
92.00	442.0
93.00	2273.0
98.00	1663.0
99.00	1556.0
100.90	781.0
104.00	439.0
105.00	458.0
107.00	5672.0
108.10	857.0
110.00	10475.0
111.00	1655.0
117.00	5025.0
118.00	375.0
122.00	381.0
123.00	609.0
124.00	348.0
127.00	20016.0
128.00	1734.0
129.00	8048.0
130.00	647.0
135.00	614.0
137.00	512.0
141.00	901.0
142.00	336.0
147.00	692.0
148.00	1355.0
149.00	318.0
153.00	363.0
155.00	618.0
156.00	854.0
161.00	509.0
164.90	368.0
166.00	339.0
167.00	2230.0
168.00	1773.0
168.90	300.0
174.00	459.0
175.00	1009.0
177.00	361.0
179.00	1384.0
180.00	1252.0
181.10	539.0
185.00	734.0
186.10	5478.0
187.00	1715.0
189.00	394.0
192.00	444.0
193.00	612.0
196.00	1105.0
198.00	40216.0
199.00	2794.0
204.00	1466.0
205.10	2343.0
206.10	10588.0
207.10	1846.0
208.00	408.0
211.10	372.0
217.00	2663.0
218.00	375.0
221.00	1453.0
221.80	453.0
223.00	631.0
224.10	5589.0
225.10	1433.0
227.00	2401.0
228.00	457.0
229.00	470.0
244.10	4188.0
245.00	511.0
246.00	898.0
255.10	21152.0
256.00	3090.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

258.00	1228.0
265.00	531.0
273.00	477.0
274.00	1668.0
275.10	8749.0
276.00	1119.0
277.10	806.0
296.10	2671.0
297.00	309.0
323.10	692.0
334.10	430.0
365.00	882.0
372.10	405.0
423.10	1228.0
424.00	490.0
441.10	3406.0
442.10	21688.0
443.10	4517.0
444.10	459.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

m/z	Abundance
39.00	1300.0
50.10	4126.0
51.10	16392.0
52.00	862.0
56.00	499.0
57.00	1208.0
63.10	773.0
65.10	384.0
68.10	371.0
69.00	20168.0
73.00	423.0
74.10	2246.0
75.00	3429.0
76.00	1133.0
77.10	24808.0
78.10	1807.0
79.00	1689.0
80.00	1273.0
81.00	1872.0
81.90	429.0
83.00	354.0
85.00	334.0
86.00	502.0
91.00	379.0
92.00	530.0
93.00	2895.0
98.00	2183.0
99.00	1974.0
101.00	1052.0
103.00	397.0
104.00	675.0
105.00	605.0
107.00	7929.0
108.00	1210.0
110.00	14751.0
111.00	2307.0
116.00	522.0
117.00	6678.0
118.00	543.0
121.90	511.0
123.00	786.0
124.00	340.0
125.00	324.0
127.00	28288.0
128.00	2061.0
129.00	11209.0
130.00	934.0
134.00	402.0
135.00	1010.0
136.00	439.0
136.90	565.0
141.00	1408.0
142.00	480.0
147.00	759.0
148.00	1856.0
149.00	455.0
153.00	398.0
154.00	321.0
155.00	863.0
156.00	1220.0
158.00	345.0
160.00	519.0
161.00	737.0
164.90	551.0
166.00	526.0
167.00	3042.0
168.00	2145.0
169.00	300.0
173.00	351.0
174.00	614.0
175.00	1216.0
175.90	341.0
177.00	508.0
179.00	2182.0
180.00	1851.0
181.10	710.0
185.00	955.0
186.10	8466.0
187.00	2337.0
189.00	566.0
191.00	321.0
192.00	661.0
193.10	872.0
196.00	1715.0
196.90	303.0
198.00	60432.0
199.00	4094.0
201.50	300.0
202.90	441.0
204.10	2168.0
205.00	3699.0
206.10	16179.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

207.10	2586.0
208.00	573.0
211.10	663.0
217.00	4032.0
218.00	551.0
221.10	2293.0
221.90	508.0
223.10	947.0
224.10	8732.0
225.10	2219.0
226.00	310.0
227.00	3639.0
228.00	507.0
229.10	654.0
237.10	462.0
242.00	436.0
243.00	599.0
244.10	6377.0
245.10	862.0
246.00	1252.0
255.10	33872.0
256.00	4969.0
257.00	420.0
258.10	2073.0
259.00	379.0
265.00	734.0
273.00	969.0
274.10	2548.0
275.10	14429.0
276.10	1887.0
277.00	1462.0
278.00	306.0
296.10	4183.0
297.00	476.0
303.00	325.0
315.00	410.0
323.10	1243.0
334.10	723.0
352.10	427.0
354.10	467.0
365.10	1889.0
372.10	653.0
403.00	339.0
422.20	353.0
423.10	2028.0
424.10	838.0
441.10	6820.0
442.10	41104.0
443.10	8009.0
444.10	841.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

m/z	Abundance
39.10	851.0
50.10	3261.0
51.10	12743.0
52.10	578.0
55.90	433.0
57.00	1001.0
63.00	555.0
65.00	340.0
69.00	15635.0
73.10	323.0
74.00	1663.0
75.10	2539.0
76.00	942.0
77.10	19288.0
78.10	1409.0
79.00	1375.0
80.00	885.0
81.00	1260.0
82.00	306.0
83.00	342.0
86.00	386.0
91.00	324.0
92.00	420.0
93.00	2315.0
98.00	1771.0
99.00	1611.0
101.00	776.0
102.90	306.0
104.00	494.0
105.00	444.0
107.00	6744.0
108.00	912.0
110.00	11611.0
111.00	1888.0
116.00	343.0
117.00	5534.0
118.00	427.0
122.00	444.0
123.00	741.0
123.90	320.0
124.90	315.0
127.00	22944.0
128.00	1752.0
129.00	9284.0
130.00	747.0
135.00	787.0
137.10	446.0
141.00	1208.0
142.00	434.0
147.00	645.0
148.00	1597.0
149.00	338.0
152.90	414.0
155.00	675.0
156.00	1152.0
160.00	364.0
161.00	679.0
165.00	456.0
166.00	362.0
167.00	2616.0
168.00	1726.0
173.00	309.0
174.00	617.0
175.00	975.0
177.00	470.0
179.00	1899.0
180.00	1537.0
181.00	542.0
185.00	885.0
186.10	7382.0
187.00	2011.0
189.00	508.0
192.00	629.0
193.00	822.0
196.00	1417.0
198.00	53544.0
199.00	3541.0
203.00	383.0
204.00	2142.0
205.00	3290.0
206.10	14081.0
207.10	2123.0
208.00	627.0
211.00	483.0
216.00	322.0
217.00	3855.0
218.00	563.0
221.10	2236.0
221.90	583.0
223.00	771.0
224.10	8300.0
225.10	1922.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

227.00	3256.0
228.10	434.0
229.00	680.0
237.10	365.0
242.10	401.0
243.10	419.0
244.10	6131.0
245.10	787.0
246.00	1194.0
255.10	31512.0
256.10	4761.0
257.00	430.0
258.00	1788.0
259.00	332.0
265.00	804.0
273.10	897.0
274.00	2426.0
275.10	13893.0
276.10	1842.0
277.00	1263.0
292.90	311.0
296.00	3957.0
297.00	523.0
303.00	465.0
315.00	502.0
323.10	1259.0
327.00	305.0
334.10	874.0
346.00	347.0
352.10	347.0
354.00	422.0
365.00	1811.0
372.10	716.0
403.10	392.0
421.00	400.0
422.10	368.0
423.10	2314.0
424.10	768.0
441.10	7393.0
442.10	46976.0
443.20	9128.0
444.10	804.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57