

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121416\
 Data File : BM008294.D
 Acq On : 14 Dec 2016 04:47
 Operator : UM/SJ
 Sample : PB95211BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK11

Quant Time: Dec 14 05:35:01 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM121416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 14 05:32:31 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	122423	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	487655	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	323503	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	667823	20.00	ng/ul	0.00
75) Chrysene-d12	21.27	240	862196	20.00	ng/ul	0.00
83) Perylene-d12	23.50	264	901986	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.24	96	19829	7.62	ng/uL	0.00
5) Phenol-d5	6.86	99	346608	36.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	209705	38.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	275531	38.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	276394	37.57	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	134458	38.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	154153	39.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	239628	33.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	336184	40.98	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	893986	41.57	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	1002715	39.46	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	112471	35.50	ng/ul	0.00
57) Fluorene-d10	15.31	176	738987	39.53	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.47	200	133398	33.56	ng/ul	0.00
70) Anthracene-d10	17.17	188	1192366	40.98	ng/ul	0.00
76) Pyrene-d10	19.47	212	1433049	43.04	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.35	264	1564978	41.32	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.39	70	7174	1.16	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121416\
Data File : BM008294.D
Acq On : 14 Dec 2016 04:47
Operator : UM/SJ
Sample : PB95211BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK11

Quant Time: Dec 14 05:35:01 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM121416.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 14 05:32:31 2016
Response via : Initial Calibration

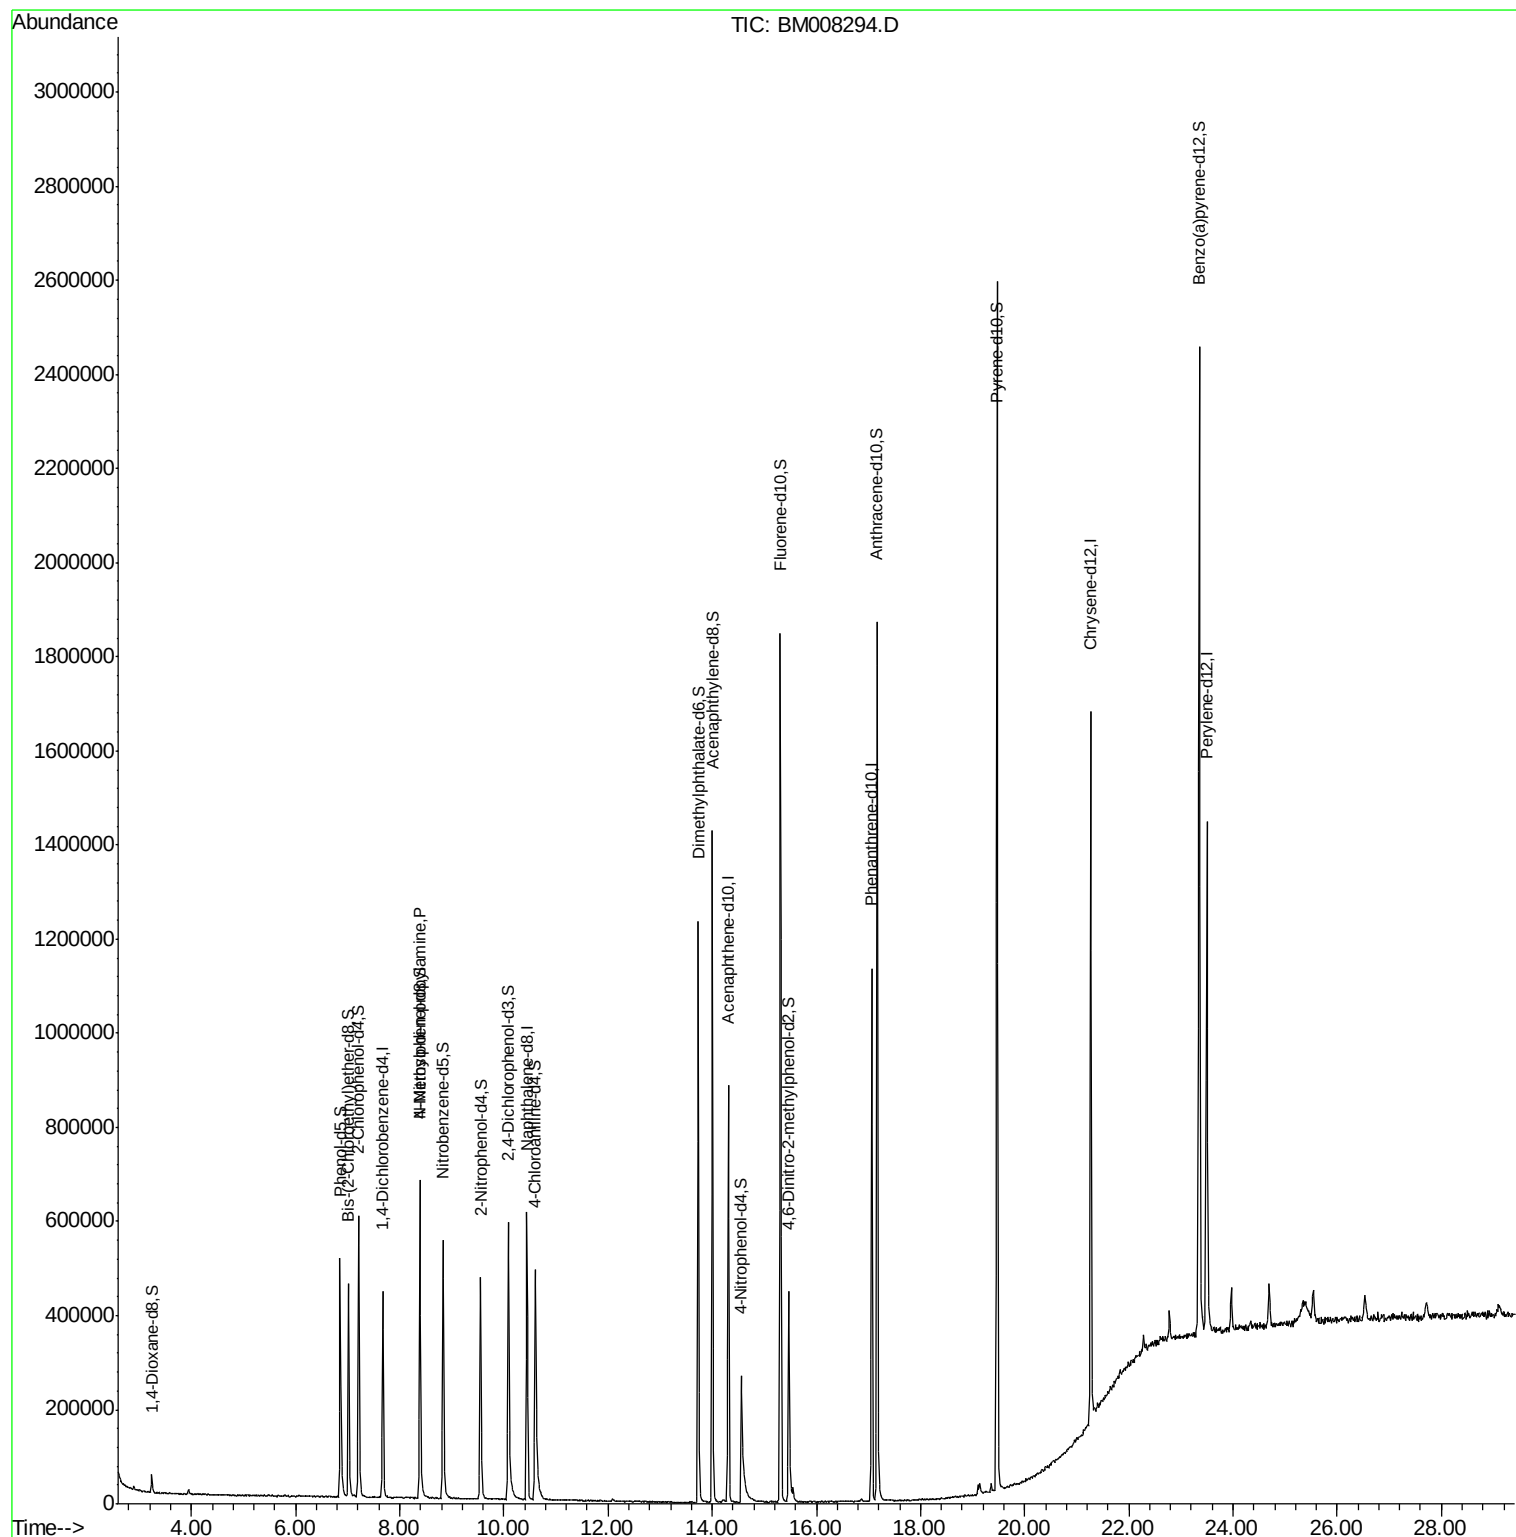

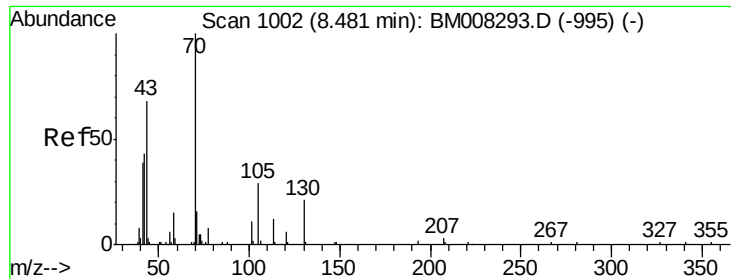

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.16 ng/ul
 RT: 8.39 min Scan# 986
 Delta R.T. -0.09 min
 Lab File: BM008294.D
 Acq: 14 Dec 2016 04:47

Instrument :
 BNA_M
 ClientSampleId :
 SBLK11

Tgt Ion: 70 Resp: 7174
 Ion Ratio Lower Upper
 70 100
 42 347.1 38.6 57.8#
 101 0.0 8.2 12.4#
 130 0.0 16.6 24.8#

