

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM121417\
 Data File : BM013433.D
 Acq On : 15 Dec 2017 10:09
 Operator : SJ/JU
 Sample : I6778-05
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 15 12:05:01 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 15 04:56:09 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	239531	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	1067067	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	629514	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1460412	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	1499791	20.00	ng/ul	0.00
83) Perylene-d12	23.48	264	1275404	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	16273	3.36	ng/uL	0.00
5) Phenol-d5	6.85	99	454614	21.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	273545	23.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	348302	21.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	440324	24.87	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	215037	25.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	247916	27.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	448877	24.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	390730	22.78	ng/ul	0.00
43) Dimethylphthalate-d6	13.74	166	2146730	38.32	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	2257140	32.65	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	433582	44.55	ng/ul	0.00
57) Fluorene-d10	15.32	176	1741577	36.15	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	382468	41.63	ng/ul	0.00
70) Anthracene-d10	17.17	188	3243401	44.34	ng/ul	0.00
76) Pyrene-d10	19.47	212	3932254	52.63	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.34	264	3390701	52.19	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	13.78	163	275943	5.150	ng/ul# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM121417\
Data File : BM013433.D
Acq On : 15 Dec 2017 10:09
Operator : SJ/JU
Sample : I6778-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Dec 15 12:05:01 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 15 04:56:09 2017
Response via : Initial Calibration

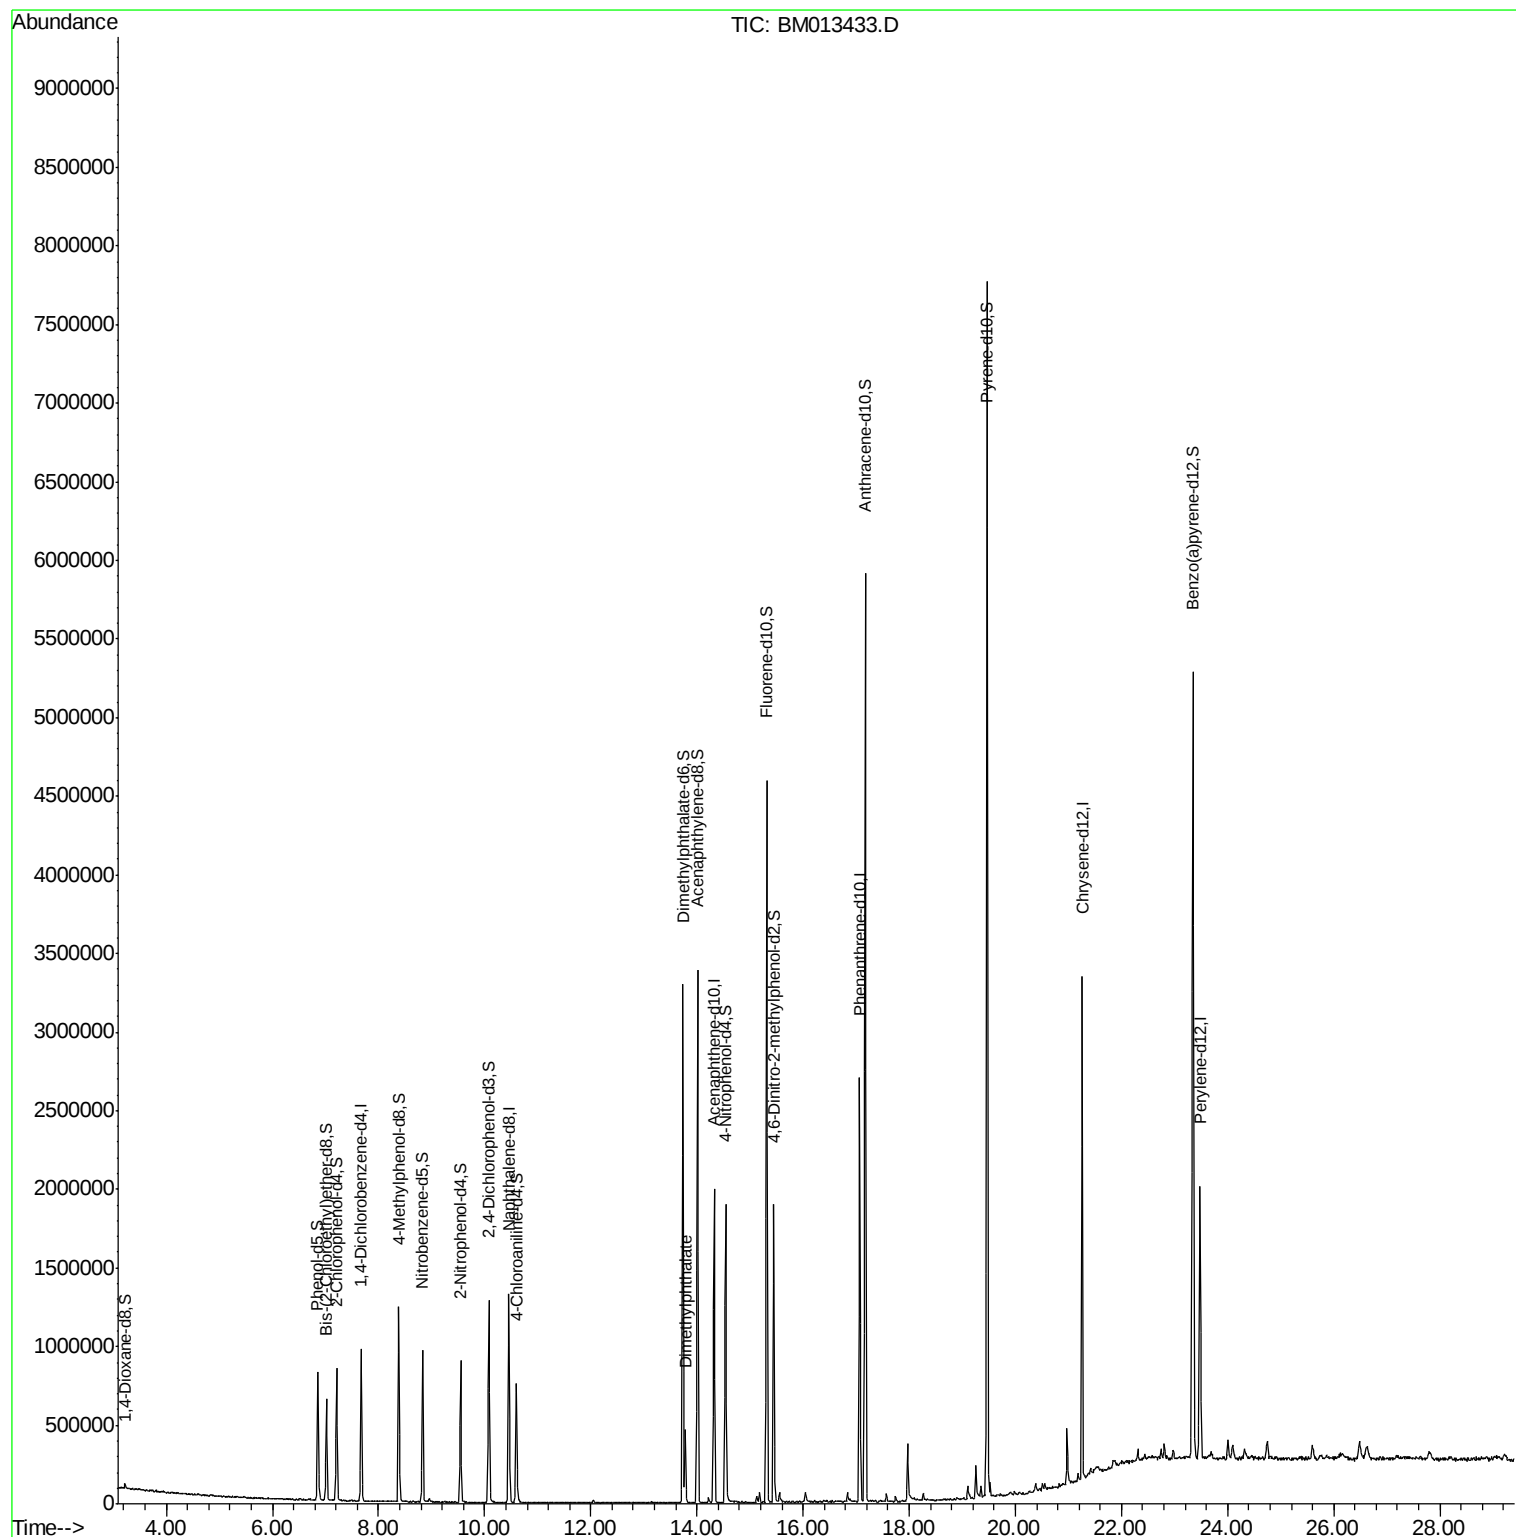


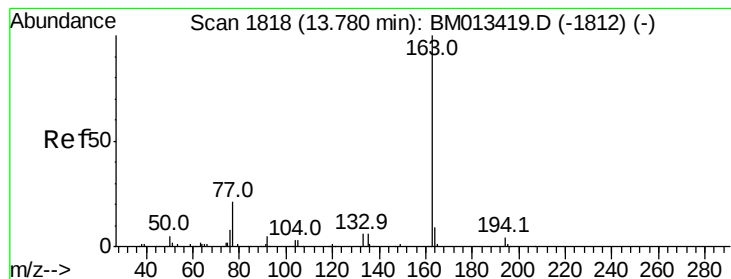

#44
 Dimethylphthalate
 Concen: 5.150 ng/ul
 RT: 13.78 min Scan# 1818
 Delta R.T. -0.01 min
 Lab File: BM013433.D
 Acq: 15 Dec 2017 10:09

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:163 Resp: 275943
 Ion Ratio Lower Upper
 163 100
 194 3.4 3.5 5.3#
 164 9.6 8.2 12.4

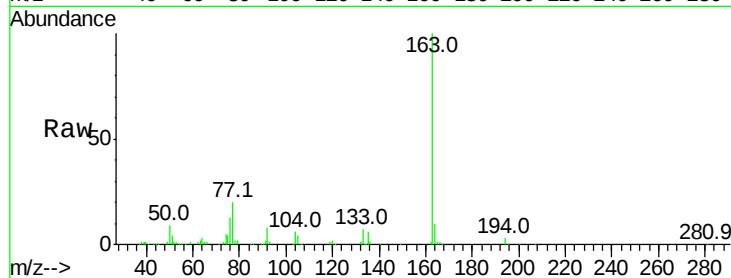

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

