


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM121417\
Data File : BM013412.D
Acq On : 14 Dec 2017 21:08
Operator : SJ/JU
Sample : I6900-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 19 17:27:34 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 15 04:56:09 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
F9C08

Manual Integrations
APPROVED

Sohil
12/15/2017 6:48:44 PM

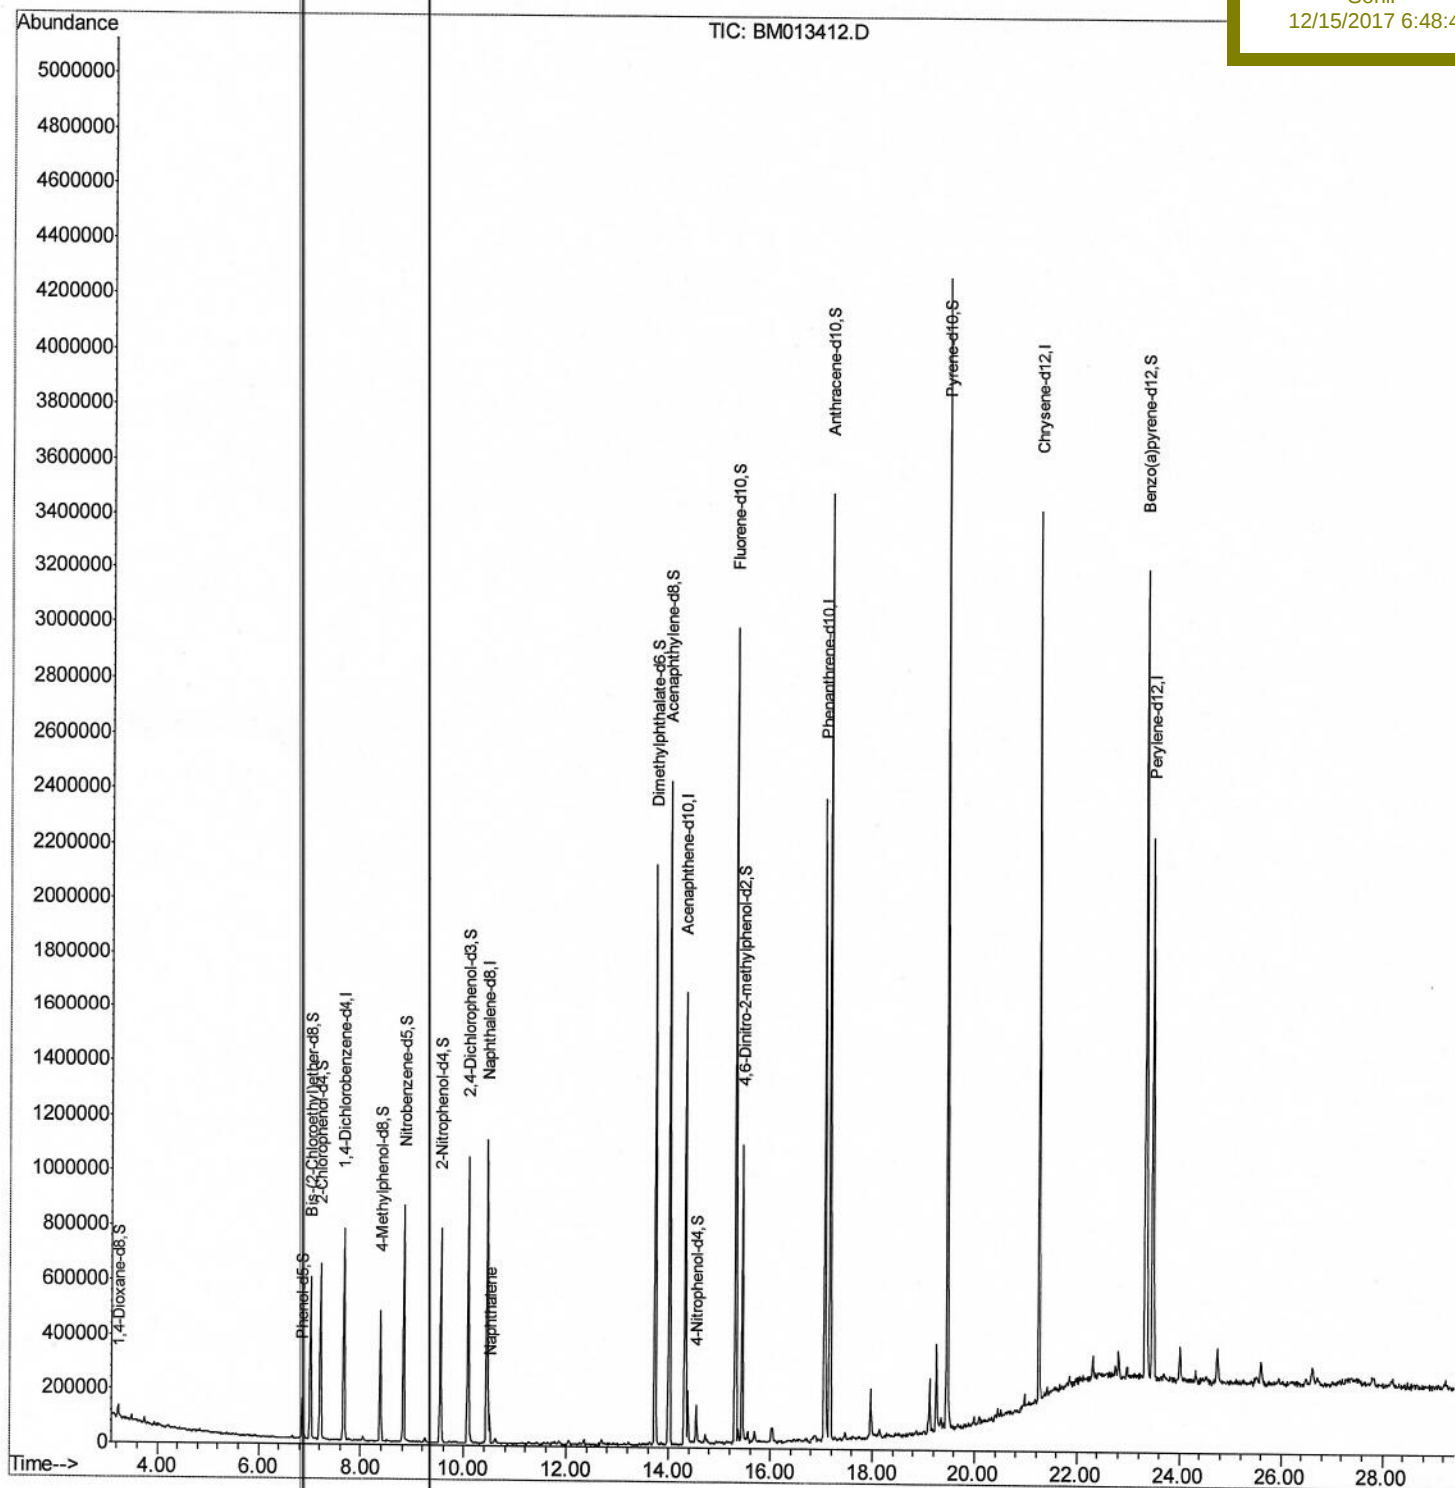

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121417\
Quantitation Report (Qedit)




Data File : BM013412.D
Acq On : 14 Dec 2017 21:08
Operator : SJ/JU
Sample : I6900-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 15 04:57:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVQA CALIBRATION
QLast Update : Fri Dec 15 04:56:09 2017
Response via : Initial Calibration

Instrument :
BNA_M
Client Sampled :
F9C08

Manual Integrations
APPROVED

Sohil
12/15/2017 6:48:44 PM

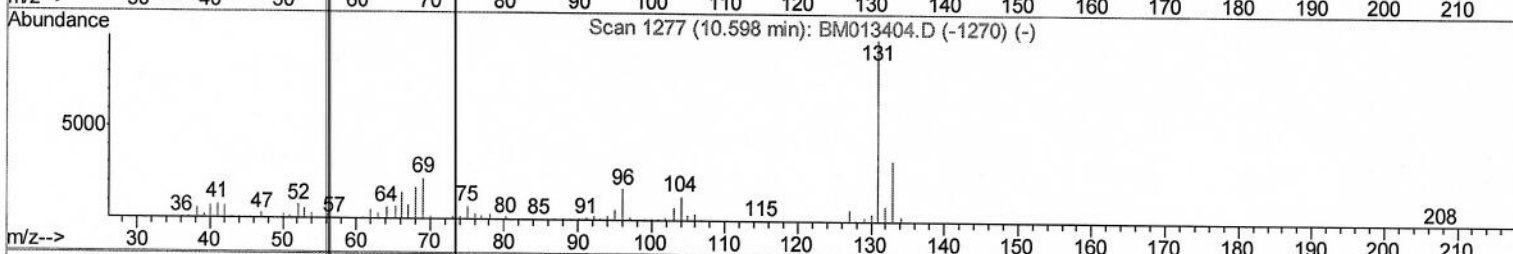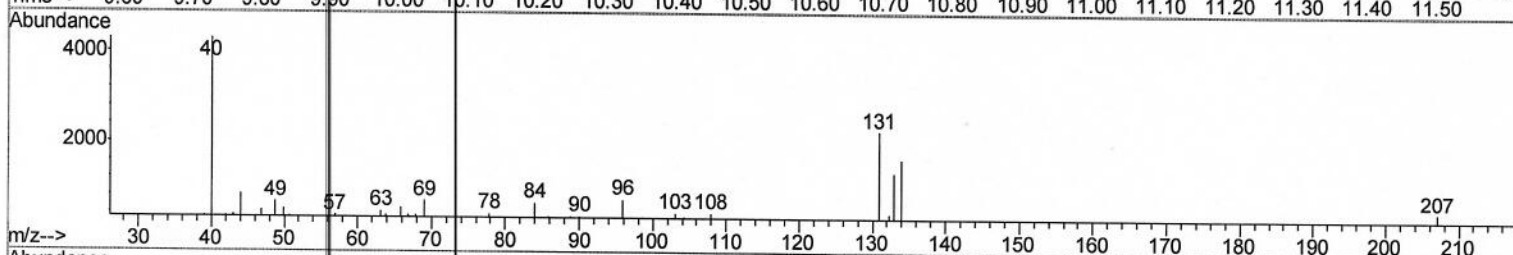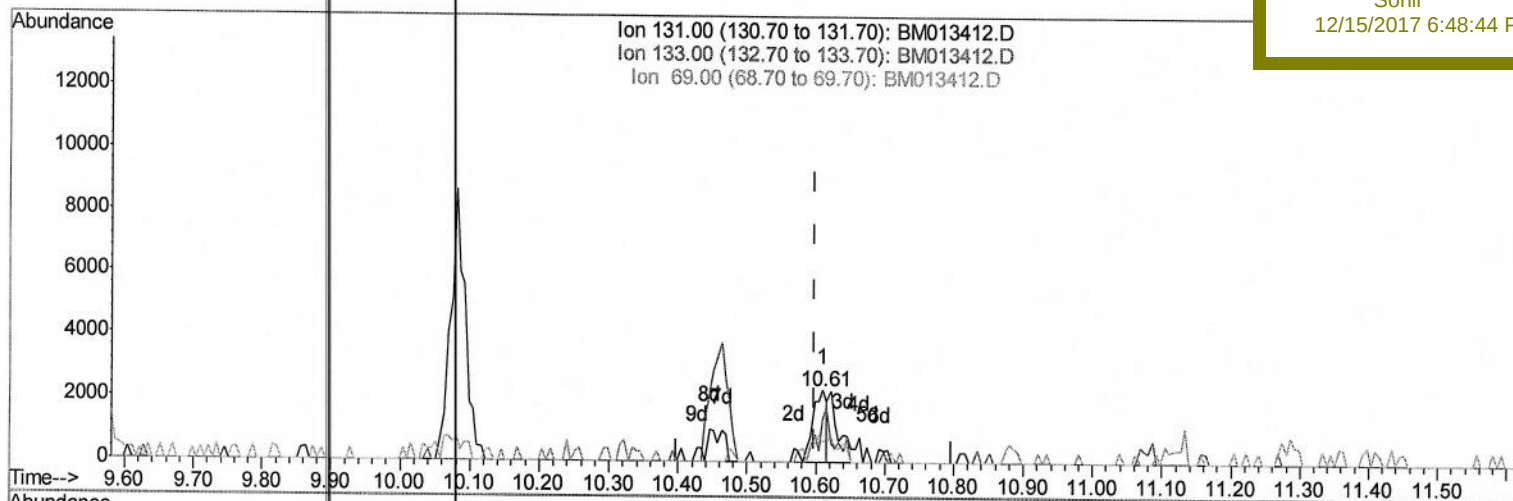

TIC: BM013412.D

(29) 4-Chloroaniline-d4 (S)
10.610min (+0.012) 0.24ng/ul
response 3284

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	59.74#
69.00	24.30	29.87#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121417\

Quantitation Report (Qedit)

Data File : BM013412.D

Acq On : 14 Dec 2017 21:08

Operator : SJ/JU

Sample : I6900-09

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 15 04:57:03 2017

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M

Quant Title : SVQA CALIBRATION

QLast Update : Fri Dec 15 04:56:09 2017

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




F9C08

Manual Integrations

APPROVED

Sohil

12/15/2017 6:48:44 PM

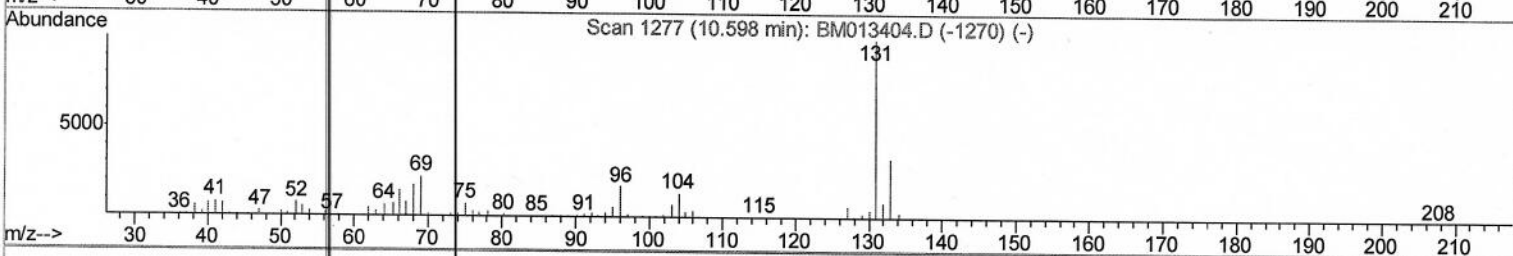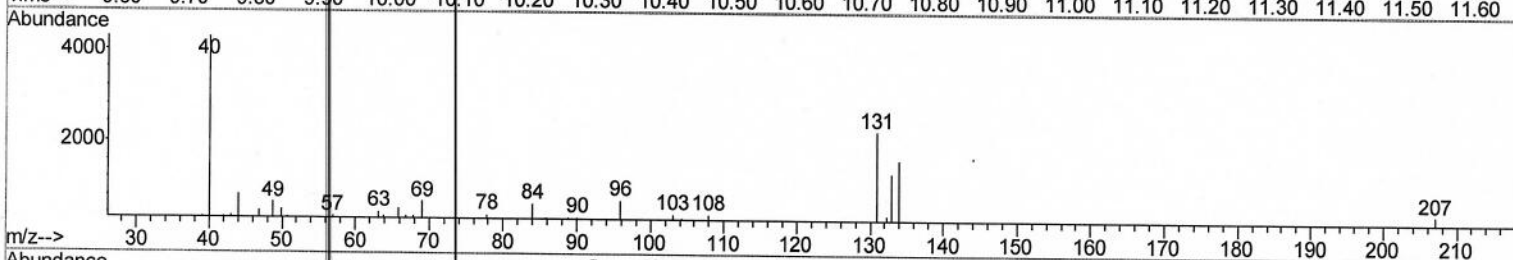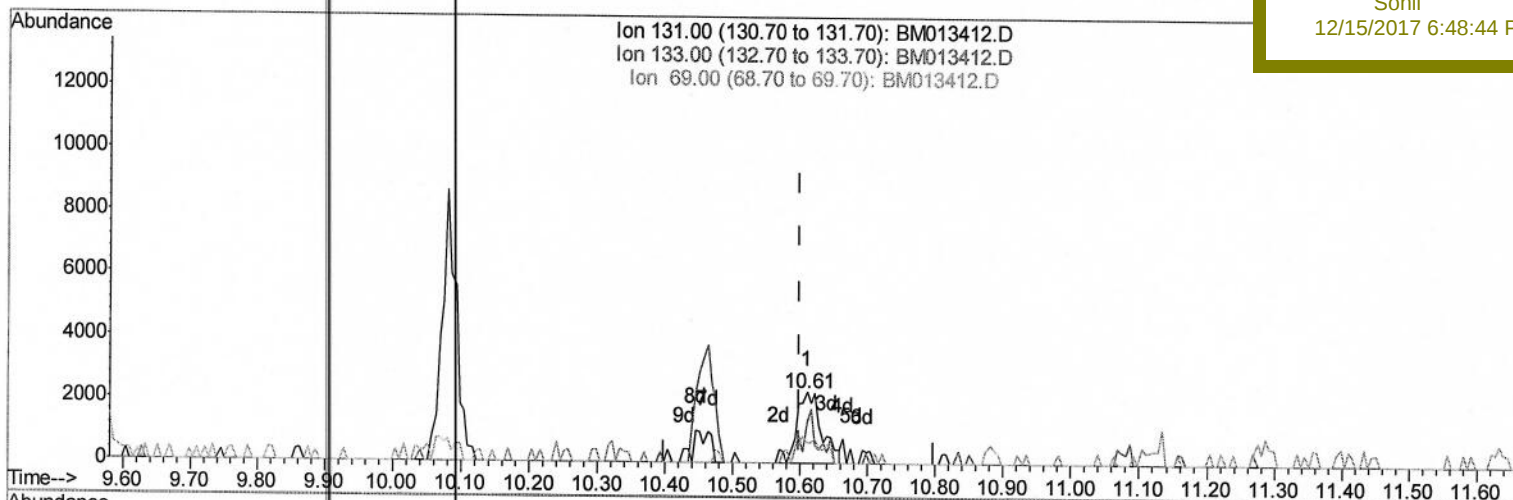

TIC: BM013412.D

(29) 4-Chloroaniline-d4 (S)

10.610min (+0.012) 0.40ng/ul m

response 5647

Ion	Exp%	Act%
-----	------	------

131.00	100	100
--------	-----	-----

133.00	31.40	59.74#
--------	-------	--------

69.00	24.30	29.87#
-------	-------	--------

0.00	0.00	0.00
------	------	------

JU 12/15/17

Data Path : \\74.0.250.170\SVASRV\HPCHEM1\BNA M\DATA\BM121417\
 Data File : BM013412.D
 Acq On : 14 Dec 2017 21:08
 Operator : SJ/JU
 Sample : I6900-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 F9C08

Quant Time: Dec 19 17:27:34 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 15 04:56:09 2017
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 12/15/2017 6:48:44 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	194279	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	868733	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	536392	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1289719	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	1532641	20.00	ng/ul	0.00
83) Perylene-d12	23.48	264	1433507	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	22846	5.82	ng/uL	0.00
5) Phenol-d5	6.85	99	82881	4.93	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.02	67	257107	26.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	269933	20.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	172372	12.00	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	184717	26.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	205757	27.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	355165	23.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.61	131	5647m	0.40	ng/ul	0.01
43) Dimethylphthalate-d6	13.73	166	1312835	27.50	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	1594545	27.07	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	33830	4.08	ng/ul	0.00
57) Fluorene-d10	15.32	176	1114158	27.14	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	207822	25.61	ng/ul	0.00
70) Anthracene-d10	17.17	188	1800183	27.87	ng/ul	0.00
76) Pyrene-d10	19.47	212	2078094	27.22	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.34	264	2003993	27.44	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
28) Naphthalene	10.50	128	77871	1.742	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed