

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM121417\
 Data File : BM013417.D
 Acq On : 15 Dec 2017 00:06
 Operator : SJ/JU
 Sample : I6778-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9A69

Quant Time: Dec 15 05:46:46 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 15 04:56:09 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	195479	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	844769	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	519412	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1226765	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	1390660	20.00	ng/ul	0.00
83) Perylene-d12	23.48	264	1269473	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	29484	7.47	ng/uL	0.00
5) Phenol-d5	6.86	99	680186	40.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	408736	42.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	548860	41.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	616204	42.65	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	306574	45.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	345642	48.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	640555	43.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	806796	59.41	ng/ul	0.00
43) Dimethylphthalate-d6	13.74	166	2478016	53.61	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	2869302	50.31	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	409816	51.03	ng/ul	0.00
57) Fluorene-d10	15.32	176	2056314	51.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	396791	51.42	ng/ul	0.00
70) Anthracene-d10	17.17	188	3423796	55.73	ng/ul	0.00
76) Pyrene-d10	19.47	212	3950190	57.02	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.34	264	3689852	57.06	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.88	94	40072	2.397 ng/ul	93
44) Dimethylphthalate	13.78	163	382770	8.658 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM121417\
Data File : BM013417.D
Acq On : 15 Dec 2017 00:06
Operator : SJ/JU
Sample : I6778-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9A69

Quant Time: Dec 15 05:46:46 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 15 04:56:09 2017
Response via : Initial Calibration

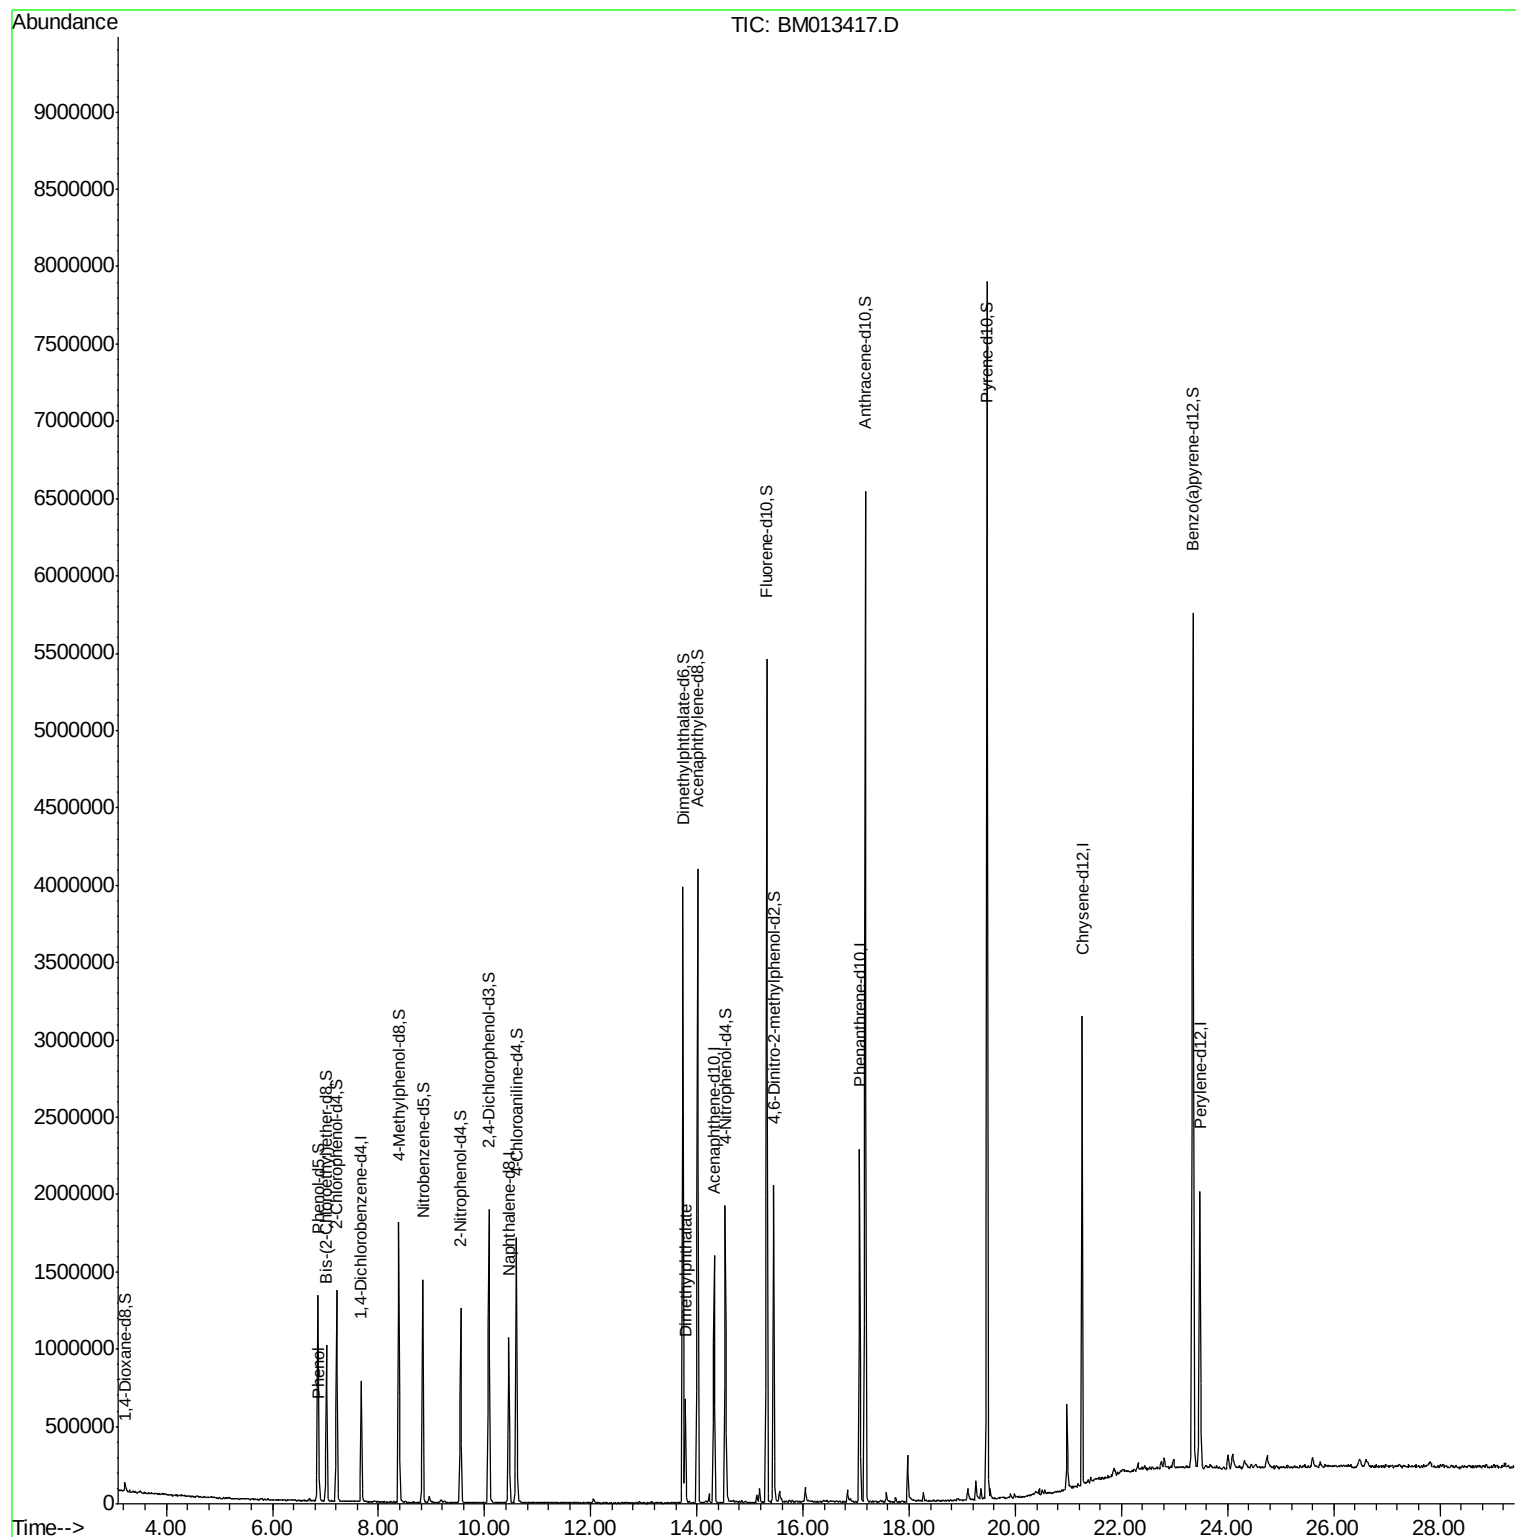

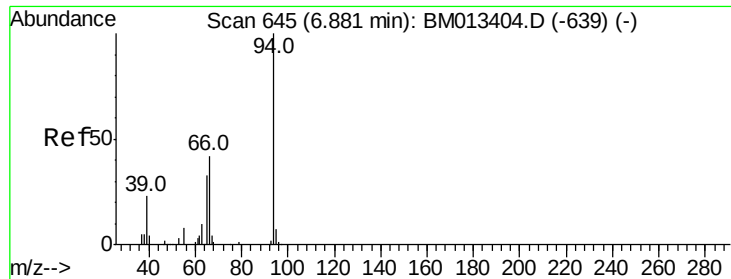





#6

Phenol

Concen: 2.397 ng/ul
 RT: 6.88 min Scan# 645
 Delta R.T. -0.01 min
 Lab File: BM013417.D
 Acq: 15 Dec 2017 00:06

Instrument :
 BNA_M
 ClientSampleId :
 F9A69

Tot Ion: 94 Resp: 40072
 Ion Ratio Lower Upper
 94 100
 65 31.2 28.2 42.4
 66 53.7 47.2 70.8

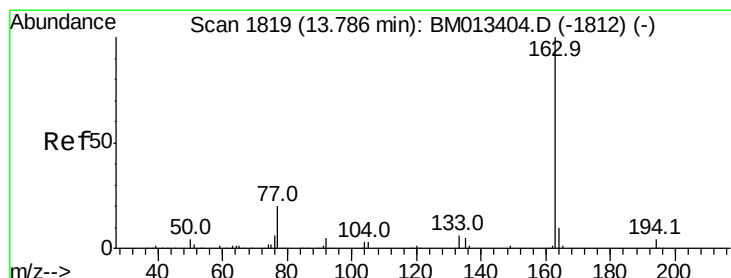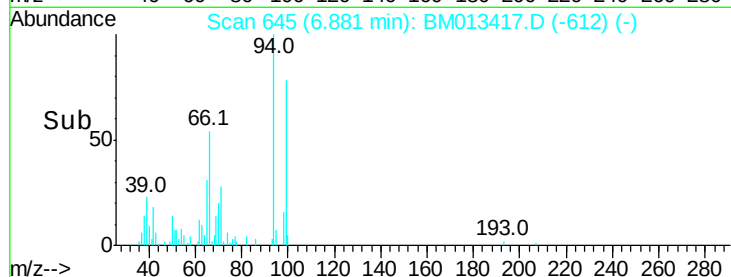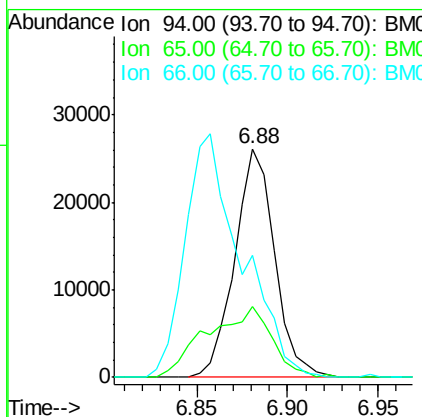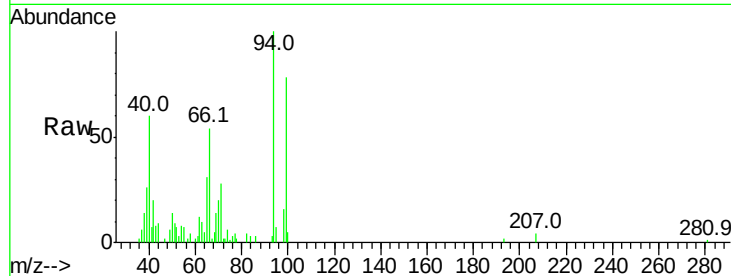

#44

Dimethylphthalate

Concen: 8.658 ng/ul
 RT: 13.78 min Scan# 1818
 Delta R.T. -0.01 min
 Lab File: BM013417.D
 Acq: 15 Dec 2017 00:06

Tgt Ion: 163 Resp: 382770
 Ion Ratio Lower Upper
 163 100
 194 4.1 3.5 5.3
 164 9.2 8.2 12.4

