

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121417\
 Data File : BM013421.D
 Acq On : 15 Dec 2017 03:03
 Operator : SJ/JU
 Sample : I6775-18 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9A63

Manual Integrations
 APPROVED

Sohil
 12/15/2017 6:48:53 PM

Quant Time: Dec 15 07:22:20 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 15 05:52:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	236770	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	1046954	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	620834	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1331879	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	1147748	20.00	ng/ul	0.00
83) Perylene-d12	23.48	264	892222	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.24	96	1197	0.25	ng/uL	0.01
5) Phenol-d5	6.86	99	35981	1.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	22935	1.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	31105	1.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	31371	1.79	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	16981	2.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	16659	1.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	29255	1.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	22343	1.33	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	117658	2.13	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	135326	1.98	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	9950	1.04	ng/ul	0.02
57) Fluorene-d10	15.32	176	94742	1.99	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	8790	1.05	ng/ul	0.00
70) Anthracene-d10	17.16	188	152144	2.28	ng/ul	0.00
76) Pyrene-d10	19.46	212	146007	2.55	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.34	264	92836	2.04	ng/ul	0.00

Target Compounds

					Qvalue	
47) Acenaphthylene	14.04	152	104445	1.655	ng/ul#	97
68) Pentachlorophenol	16.72	266	50763	5.083	ng/ul	92
69) Phenanthrene	17.11	178	131692	1.740	ng/ul	99
71) Anthracene	17.20	178	176935	2.288	ng/ul	99
74) Fluoranthene	19.13	202	810886	8.745	ng/ul#	93
77) Pyrene	19.49	202	1011271	14.503	ng/ul#	93
80) Benzo(a)anthracene	21.24	228	591044	8.116	ng/ul	97
82) Chrysene	21.29	228	665493	9.850	ng/ul	96
85) Benzo(b)fluoranthene	22.81	252	1538770	25.584	ng/ul#	98
86) Benzo(k)fluoranthene	22.86	252	474007m	8.374	ng/ul	
88) Benzo(a)pyrene	23.38	252	668557	12.374	ng/ul#	98
89) Indeno(1,2,3-cd)pyrene	25.70	276	488089	9.105	ng/ul#	95
91) Benzo(g,h,i)perylene	26.38	276	413438	9.777	ng/ul#	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121417\
Data File : BM013421.D
Acq On : 15 Dec 2017 03:03
Operator : SJ/JU
Sample : I6775-18 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F9A63

Manual Integrations
APPROVED

Sohil
12/15/2017 6:48:53 PM

Quant Time: Dec 15 07:22:20 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 15 05:52:21 2017
Response via : Initial Calibration

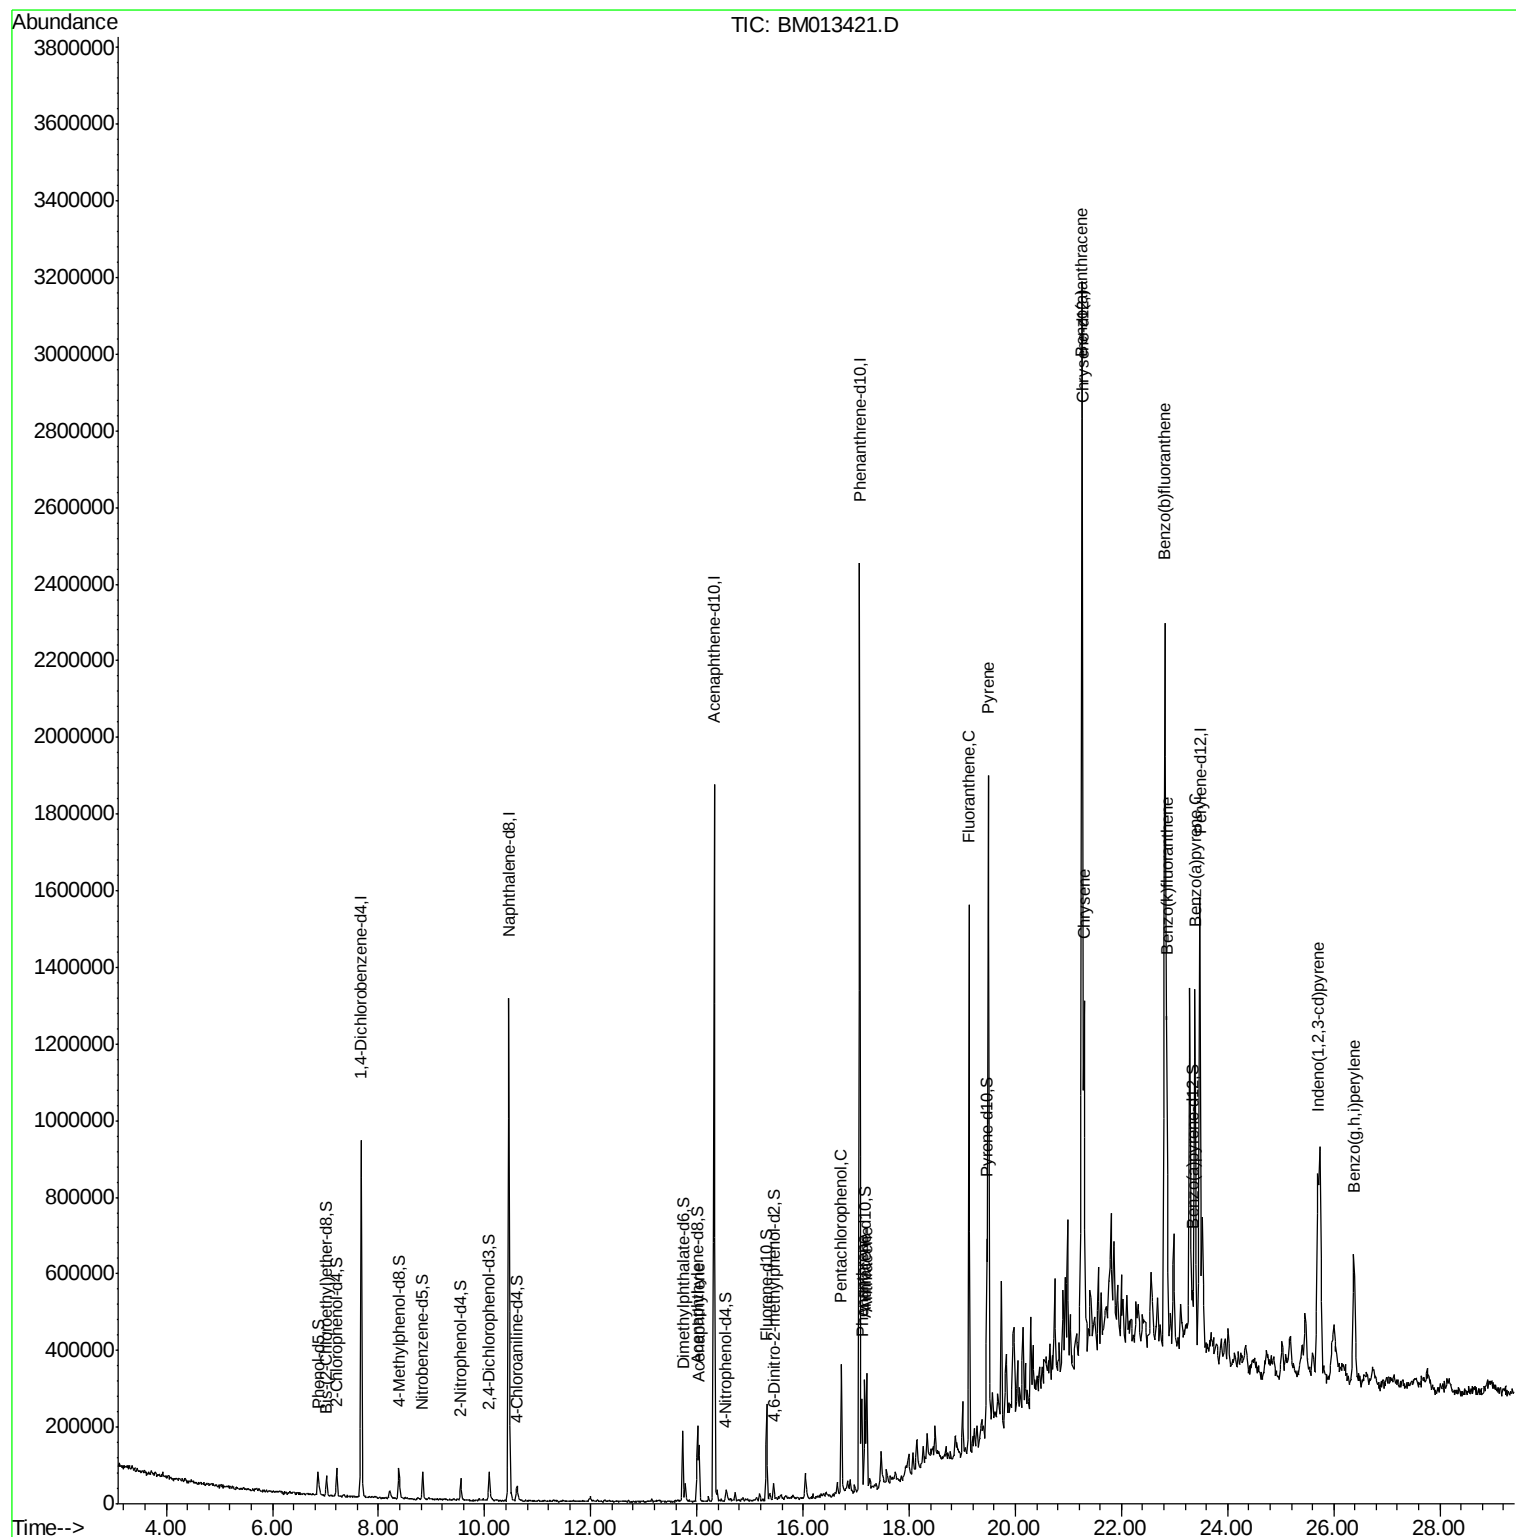

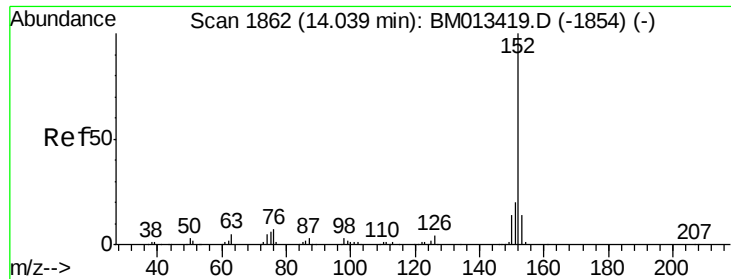

#47

Acenaphthylene

Concen: 1.655 ng/ul

RT: 14.04 min Scan# 1862

Delta R.T. 0.00 min

Lab File: BM013421.D

Acq: 15 Dec 2017 03:03

Instrument :

BNA_M





ClientSampleId :

F9A63

Tgt Ion:	152	Resp:	104445
Ion Ratio	Lower	Upper	
152	100		
151	20.9	16.3	24.5
153	15.7	10.2	15.4

Manual Integrations
APPROVED

Sohil
12/15/2017 6:48:53 PM

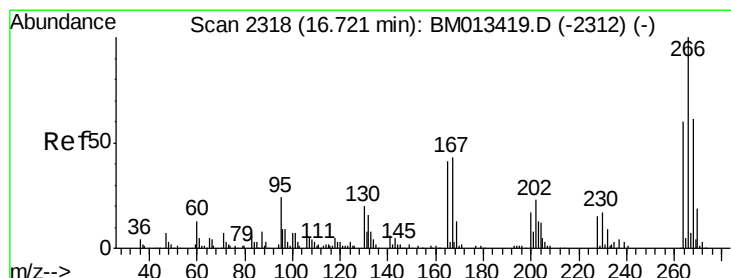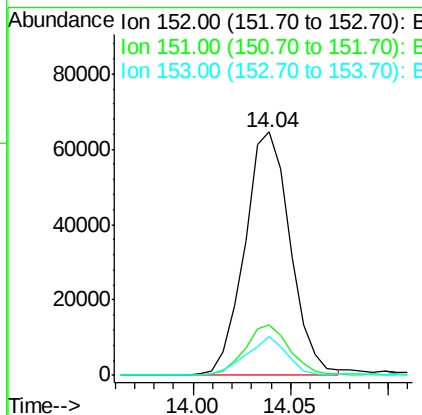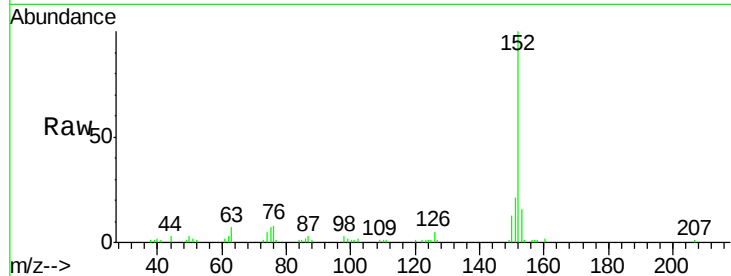

#68

Pentachlorophenol

Concen: 5.083 ng/ul




RT: 16.72 min Scan# 2318


Delta R.T. -0.00 min

Lab File: BM013421.D

Acq: 15 Dec 2017 03:03

Tgt Ion:	266	Resp:	50763
Ion Ratio	Lower	Upper	
266	100		
264	65.1	49.3	73.9
268	56.8	52.6	78.8

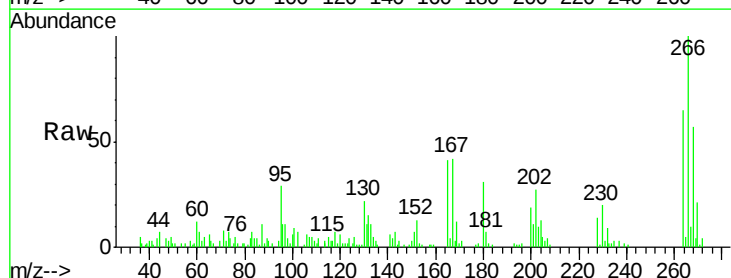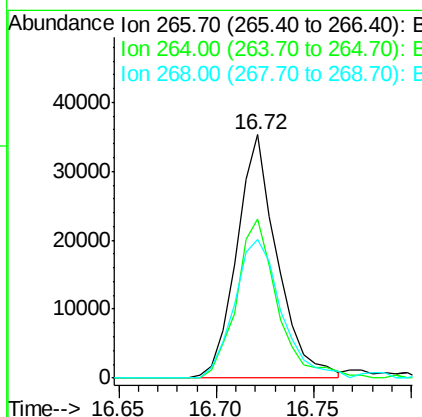



#69

Phenanthrene

Concen: 1.740 ng/ul

RT: 17.11 min Scan# 2384

Delta R.T. 0.00 min

Lab File: BM013421.D

Acq: 15 Dec 2017 03:03

Instrument :

BNA_M





ClientSampleId :

F9A63

Tgt Ion:	178	Resp:	131692
Ion Ratio	Lower	Upper	
178	100		
179	15.6	12.6	19.0
176	19.5	14.9	22.3

Manual Integrations
APPROVED

Sohil
12/15/2017 6:48:53 PM

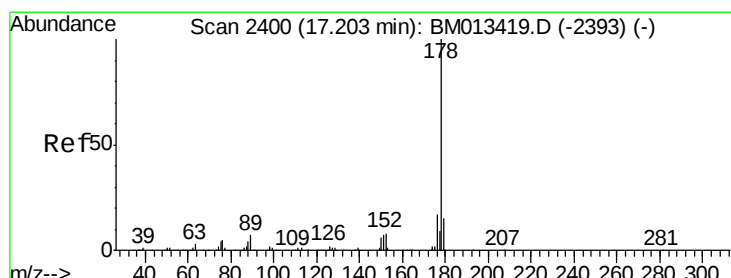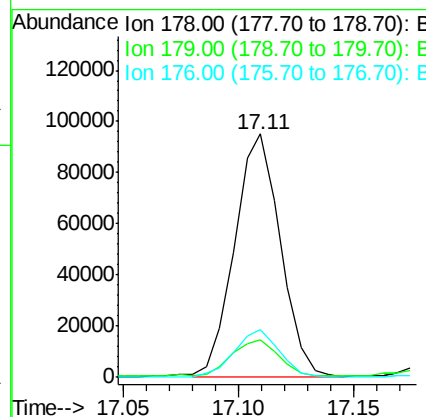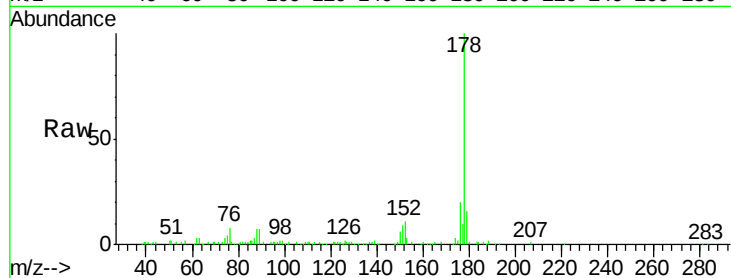

#71

Anthracene

Concen: 2.288 ng/ul




RT: 17.20 min Scan# 2399


Delta R.T. -0.01 min

Lab File: BM013421.D

Acq: 15 Dec 2017 03:03

Tgt Ion:	178	Resp:	176935
Ion Ratio	Lower	Upper	
178	100		
179	14.3	11.7	17.5
176	17.8	14.6	21.8

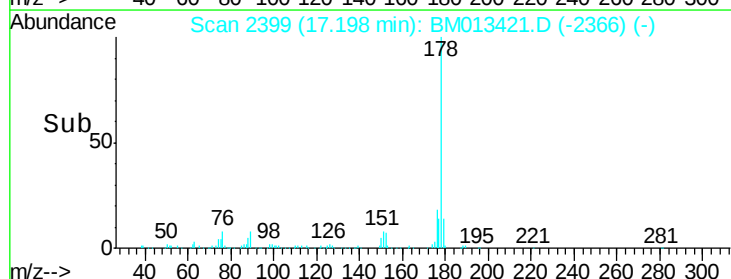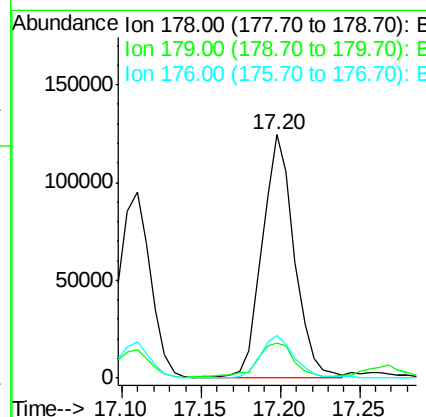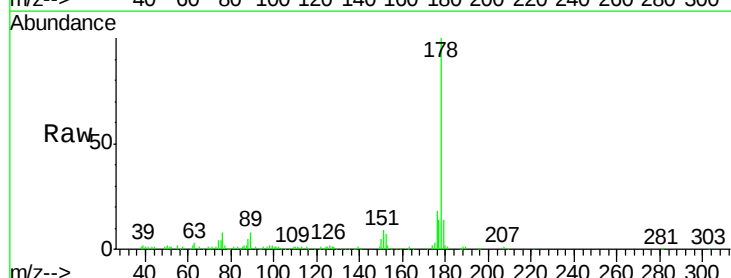

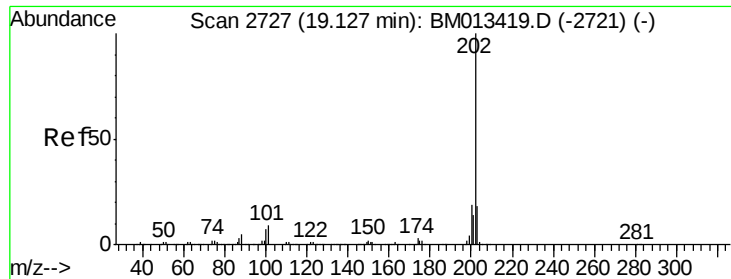





#74
 Fluoranthene
 Concen: 8.745 ng/ul
 RT: 19.13 min Scan# 2727
 Delta R.T. 0.00 min
 Lab File: BM013421.D
 Acq: 15 Dec 2017 03:03

Instrument :
 BNA_M
 ClientSampleId :
 F9A63

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	8.5	4.6	7.0#
100	6.4	3.4	5.2#




Manual Integrations
 APPROVED


Sohil
 12/15/2017 6:48:53 PM

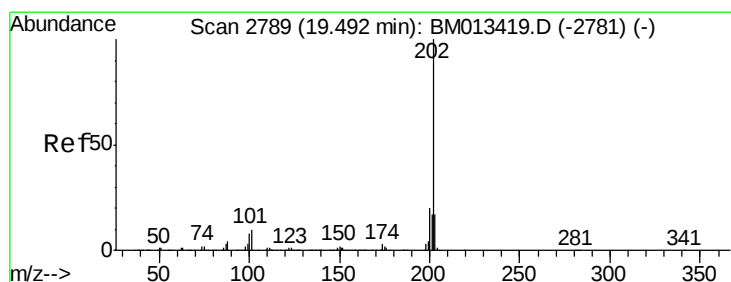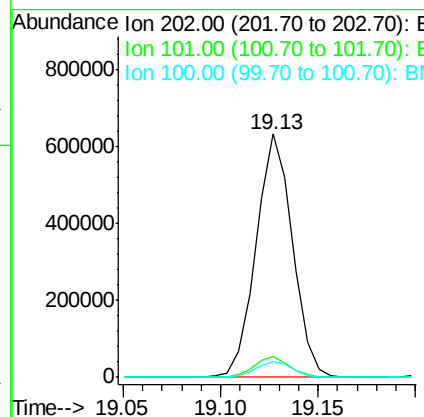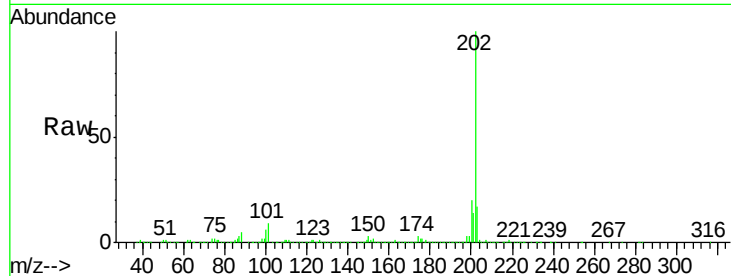

#77
 Pyrene
 Concen: 14.503 ng/ul
 RT: 19.49 min Scan# 2789
 Delta R.T. 0.00 min
 Lab File: BM013421.D
 Acq: 15 Dec 2017 03:03

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	9.6	5.1	7.7#
100	7.9	4.9	7.3#

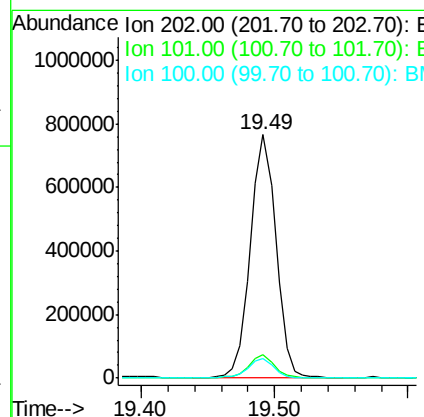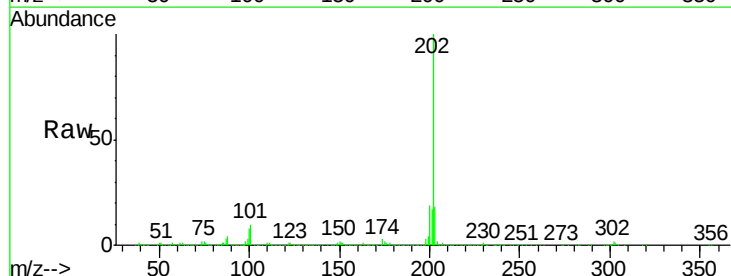

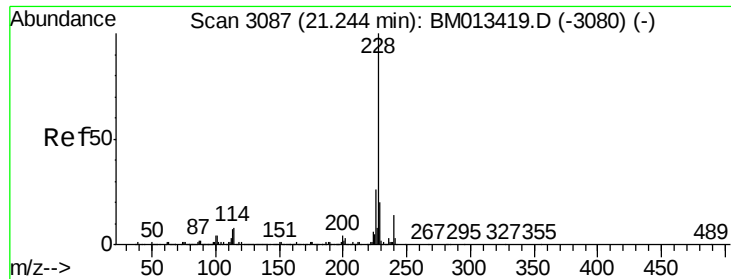





#80
Benzo(a)anthracene
Concen: 8.116 ng/ul
RT: 21.24 min Scan# 3087
Delta R.T. -0.00 min
Lab File: BM013421.D
Acq: 15 Dec 2017 03:03

Instrument :
BNA_M
ClientSampleId :
F9A63

Tgt Ion	Ratio	Lower	Upper
228	100		
229	19.7	15.4	23.0
226	28.9	21.4	32.0




Manual Integrations
APPROVED


Sohil
12/15/2017 6:48:53 PM

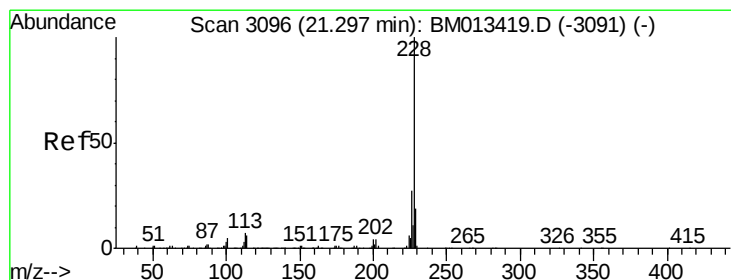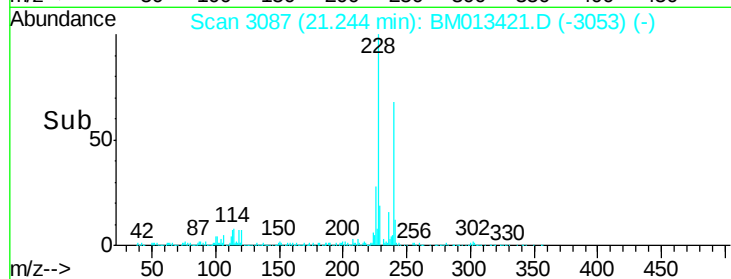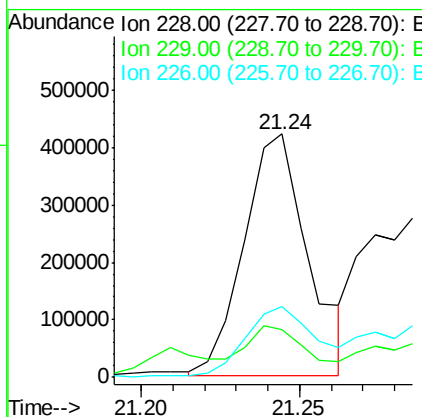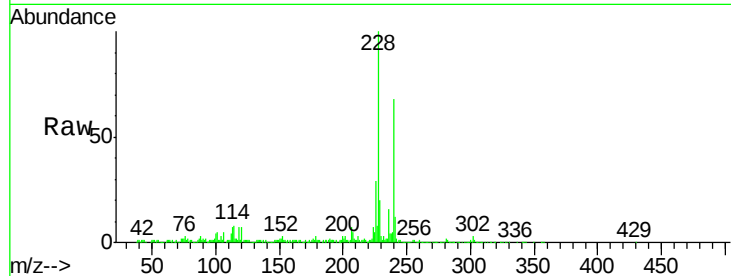

#82
Chrysene
Concen: 9.850 ng/ul
RT: 21.29 min Scan# 3095
Delta R.T. -0.01 min
Lab File: BM013421.D
Acq: 15 Dec 2017 03:03

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.3	23.4	35.2
229	22.3	15.5	23.3

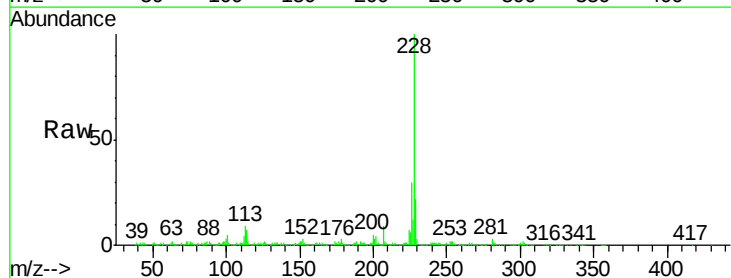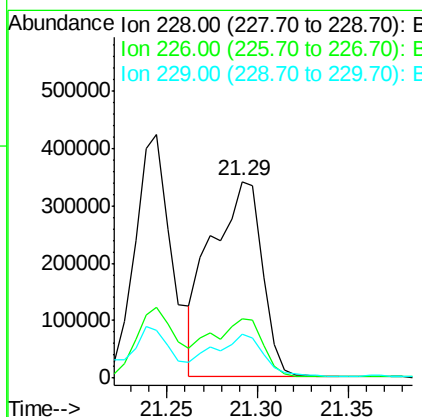

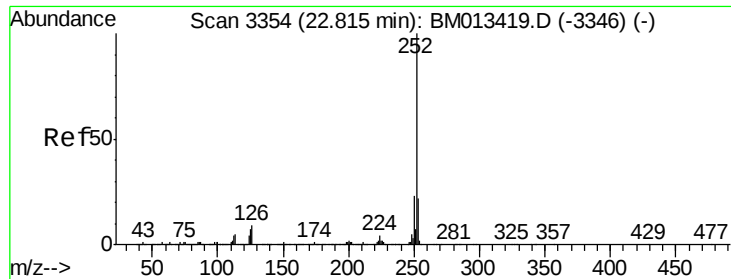





#85
Benzo(b)fluoranthene
Concen: 25.584 ng/ul
RT: 22.81 min Scan# 3354
Delta R.T. 0.00 min
Lab File: BM013421.D
Acq: 15 Dec 2017 03:03

Instrument :
BNA_M
ClientSampleId :
F9A63

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.2	17.9	26.9
125	7.5	3.6	5.4




Manual Integrations
APPROVED


Sohil
12/15/2017 6:48:53 PM

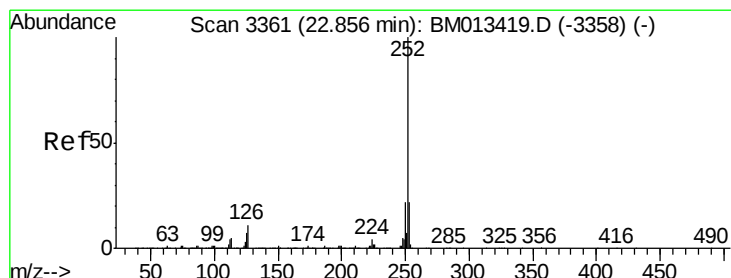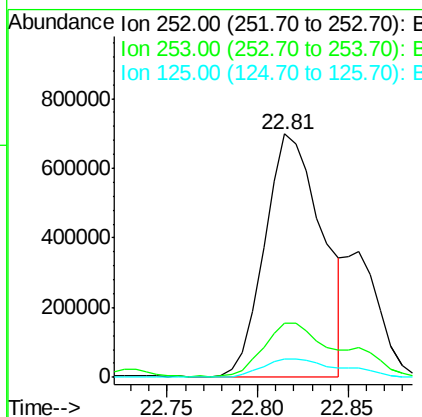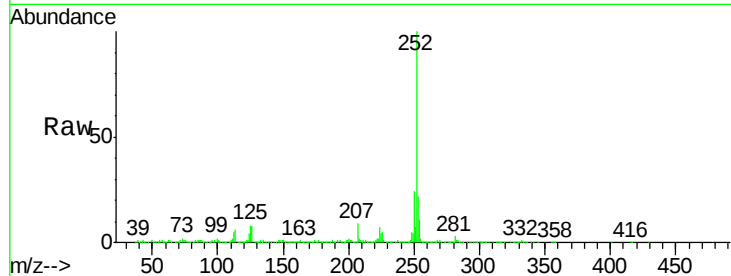

#86
Benzo(k)fluoranthene
Concen: 8.374 ng/ul m
RT: 22.86 min Scan# 3361
Delta R.T. -0.00 min
Lab File: BM013421.D
Acq: 15 Dec 2017 03:03

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.1	17.1	25.7
125	7.1	3.4	5.2

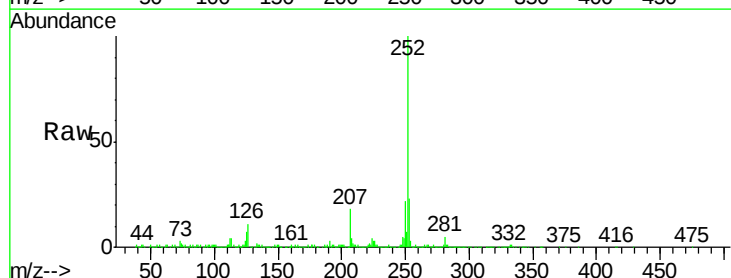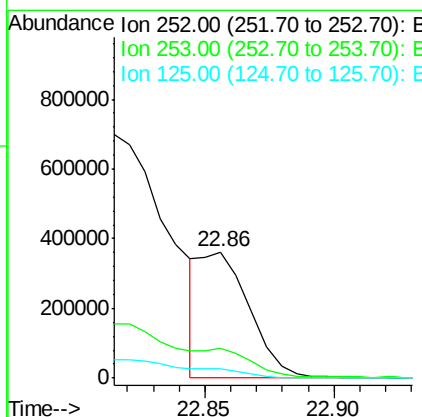

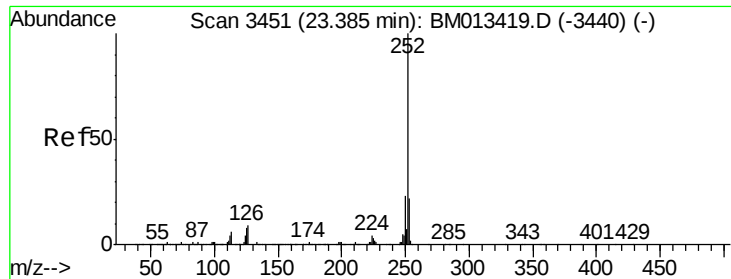

#88

Benzo(a)pyrene

Concen: 12.374 ng/ul

RT: 23.38 min Scan# 3450

Delta R.T. -0.01 min

Lab File: BM013421.D

Acq: 15 Dec 2017 03:03

Instrument :

BNA_M





ClientSampleId :

F9A63

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	668557		
253	23.5	18.2	27.2	
125	6.8	4.0	6.0#	

Manual Integrations
APPROVED

Sohil
12/15/2017 6:48:53 PM

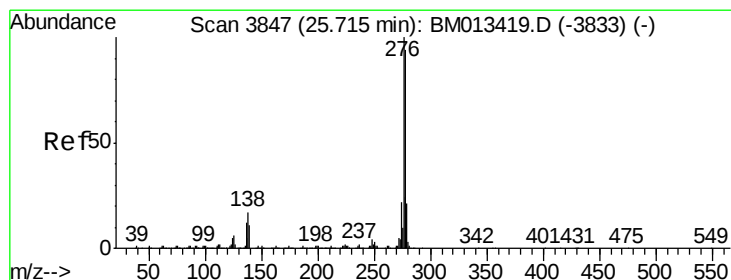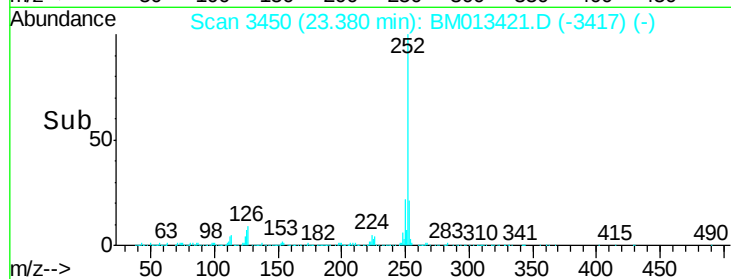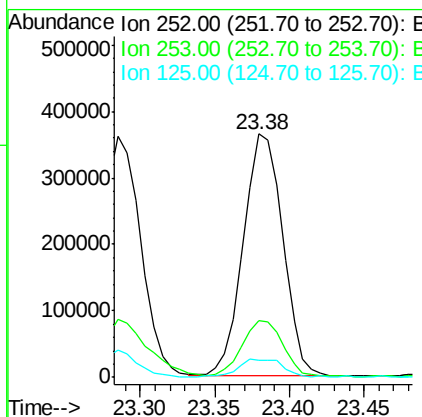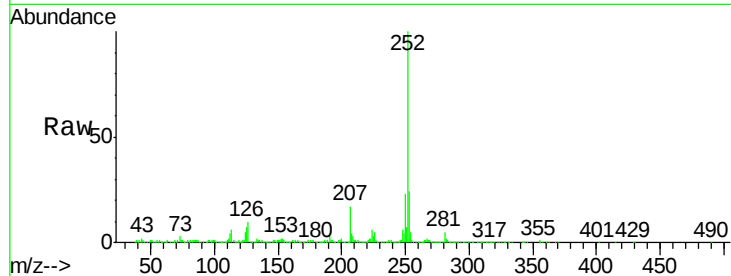

#89

Indeno(1,2,3-cd)pyrene

Concen: 9.105 ng/ul




RT: 25.70 min Scan# 3844


Delta R.T. -0.02 min

Lab File: BM013421.D

Acq: 15 Dec 2017 03:03

Tgt Ion	Ratio	Resp	Lower	Upper
276	100	488089		
138	15.6	9.3	13.9#	
277	23.5	19.9	29.9	

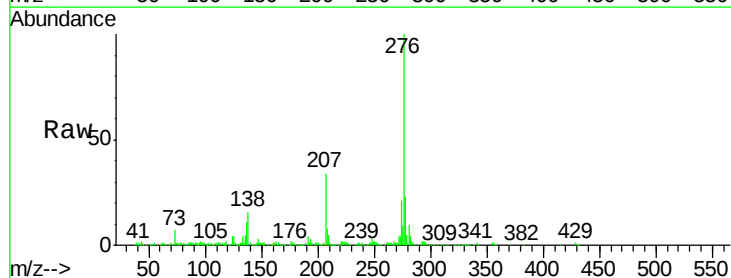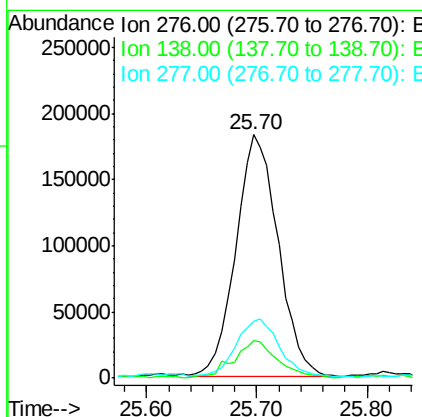

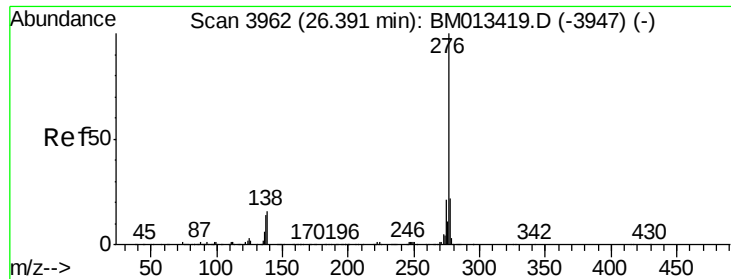

#91
 Benzo(g,h,i)perylene
 Concen: 9.777 ng/ul
 RT: 26.38 min Scan# 3960
 Delta R.T. -0.01 min
 Lab File: BM013421.D
 Acq: 15 Dec 2017 03:03

Instrument :
 BNA_M
 ClientSampleId :
 F9A63

Tgt	Ion	Ratio	Resp	Lower	Upper
276	100		413438		
138	15.8	8.5	12.7#		
277	26.5	18.6	28.0		

Manual Integrations
 APPROVED

Sohil
 12/15/2017 6:48:53 PM

