

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121515\
 Data File : BM003557.D
 Acq On : 15 Dec 2015 20:18
 Operator : UM/IZ
 Sample : PB87221BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK21

Manual Integrations
 APPROVED

MMdadoda
 12/16/2015 5:46:23 PM

Quant Time: Dec 16 05:55:20 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 16 05:49:57 2015
 Response via : Initial Calibration

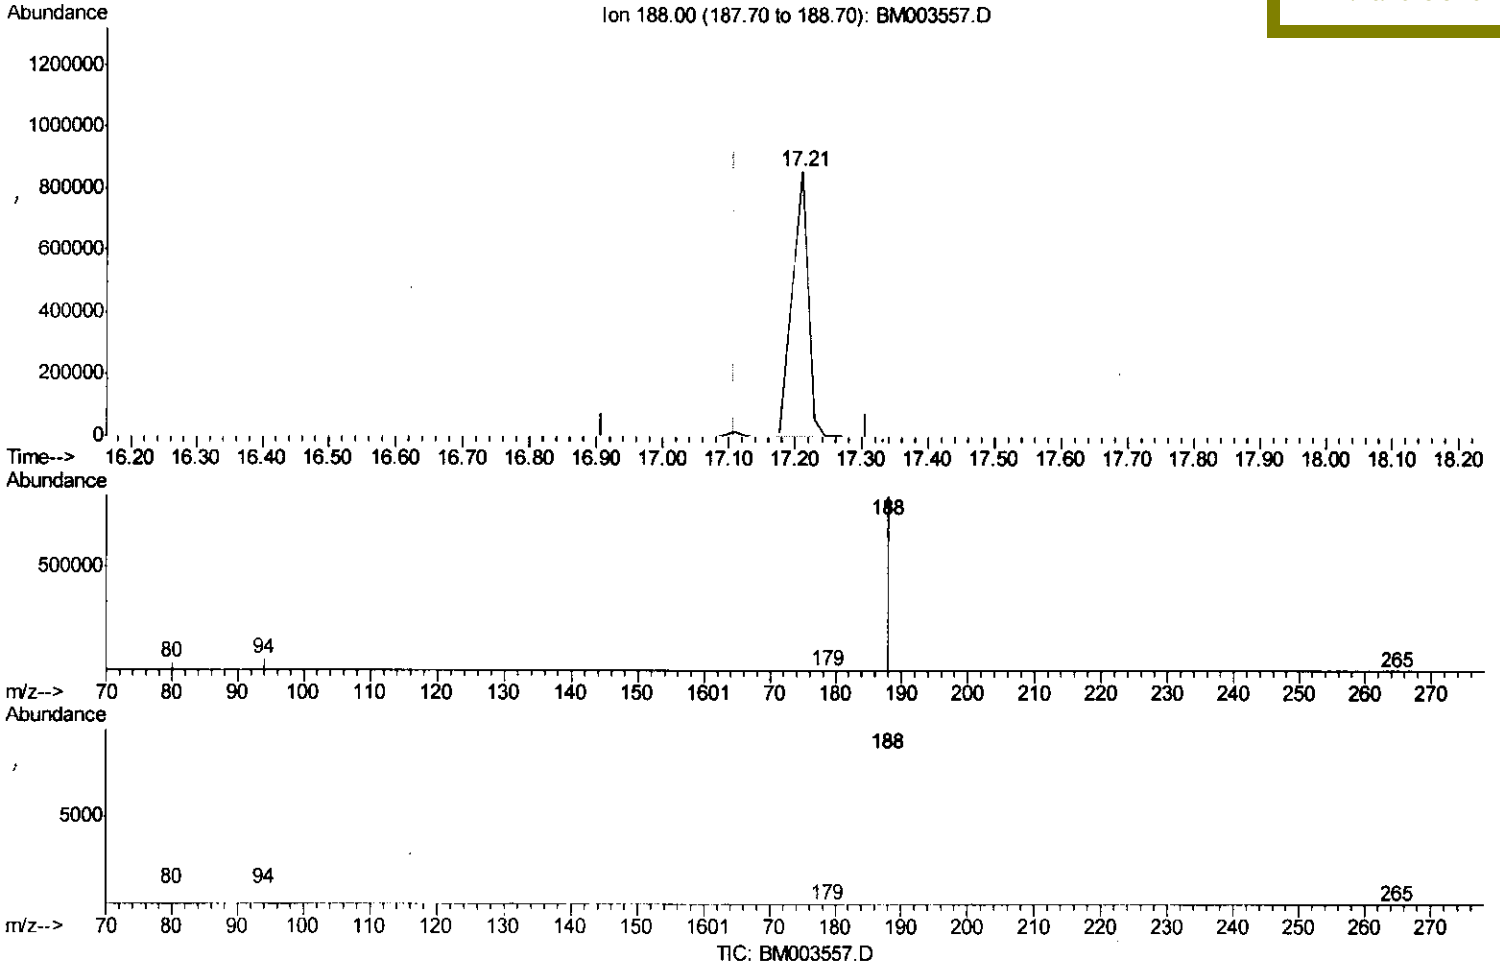

(12) Phenanthrene-d10 (I)

17.210min (+0.103) 0.40ng/ul

response 1414827

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	6.26#
80.00	11.90	4.40#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121515\
 Data File : BM003557.D
 Acq On : 15 Dec 2015 20:18
 Operator : UM/IZ
 Sample : PB87221BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK21

Manual Integrations
 APPROVED

MMdadoda
 12/16/2015 5:46:23 PM

Quant Time: Dec 16 05:55:20 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 16 05:49:57 2015
 Response via : Initial Calibration

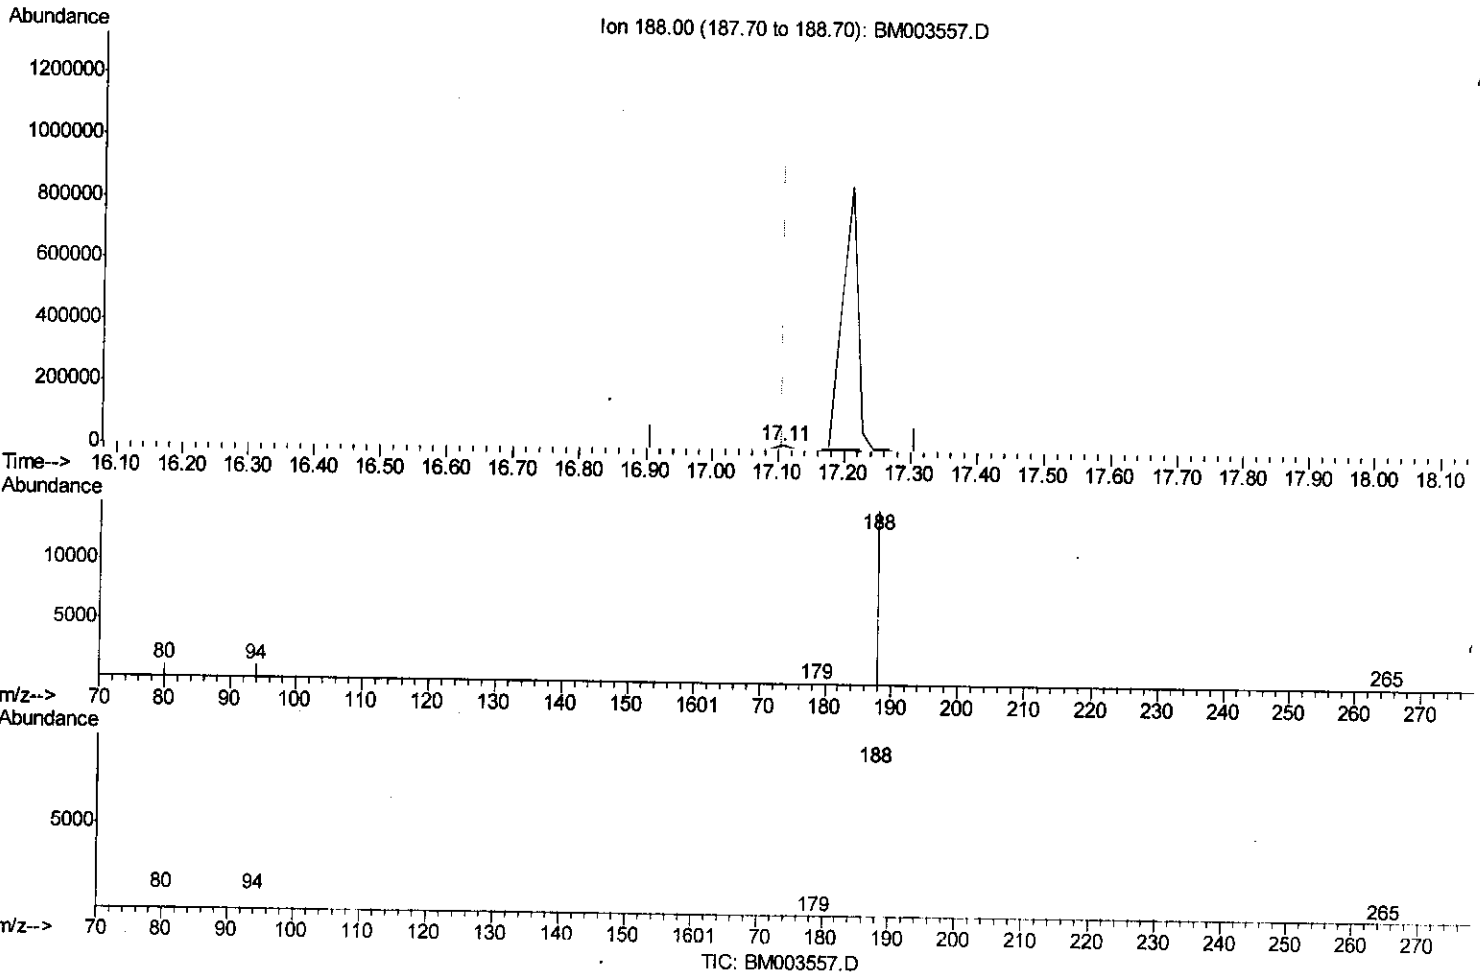

(12) Phenanthrene-d10 (I)

17.108min (+0.000) 0.40ng/ul m

response 20874

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	7.68#
80.00	11.90	7.22#
0.00	0.00	0.00

U.M
 12/17/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121515\
 Data File : BM003557.D
 Acq On : 15 Dec 2015 20:18
 Operator : UM/IZ
 Sample : PB87221BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 SBLK21

Quant Time: Dec 16 06:12:53 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 16 05:49:57 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMdadoda
 12/16/2015 5:46:23 PM

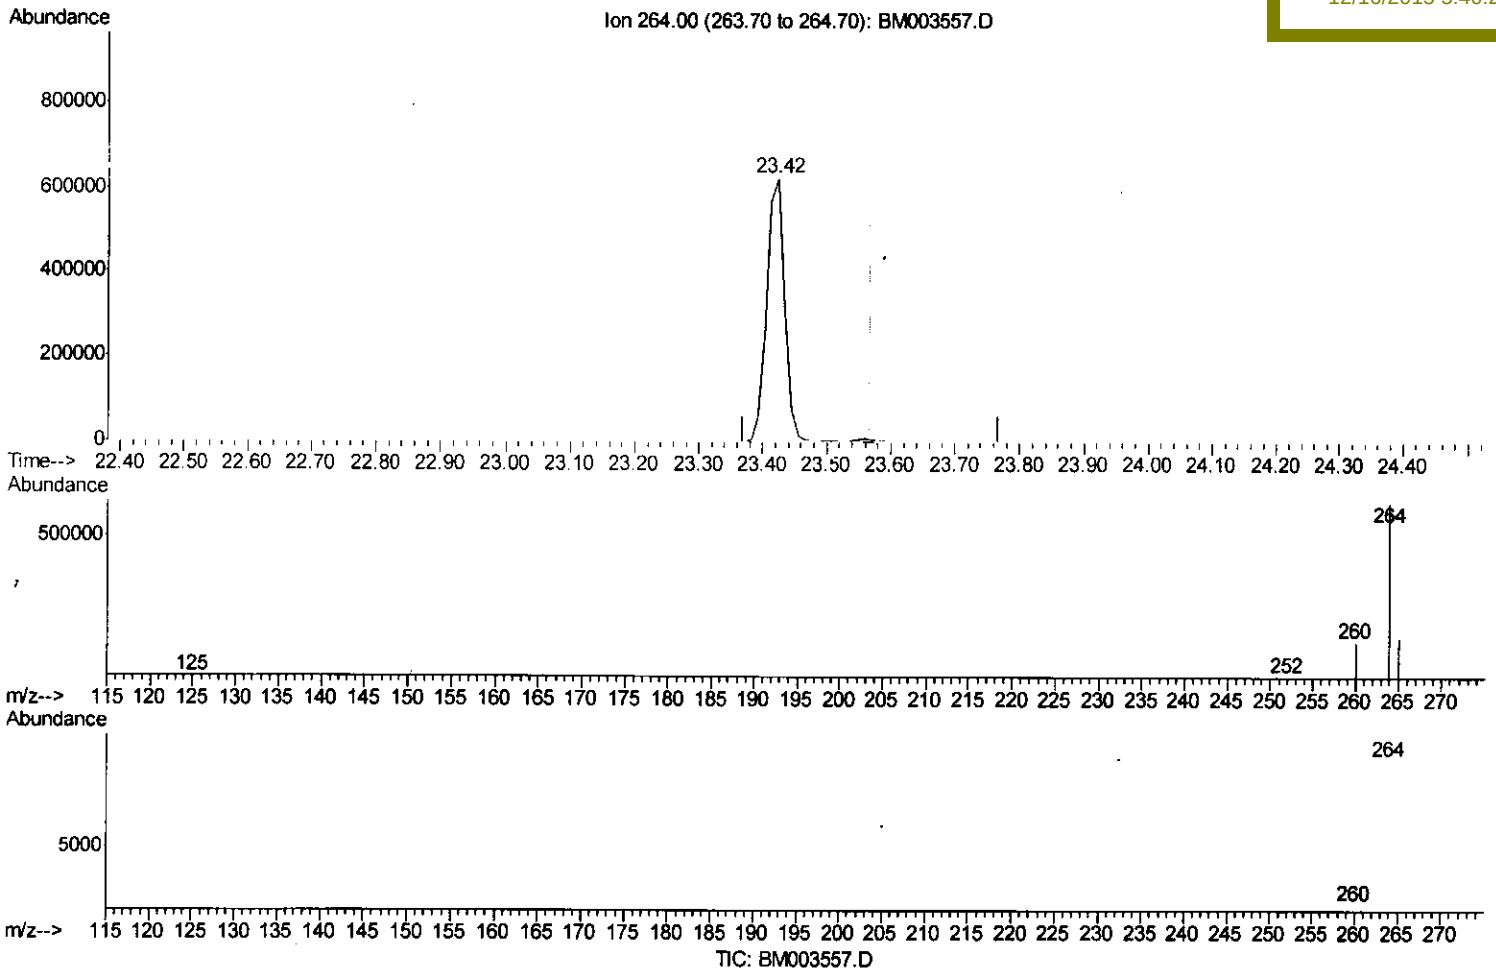

(22) Perylene-d12 (I)

23.423min (-0.146) 0.40ng/ul

response 1196638

Ion	Exp%	Act%
-----	------	------

264.00	100	100
--------	-----	-----

260.00	25.60	20.30#
--------	-------	--------

265.00	38.20	22.49#
--------	-------	--------

0.00	0.00	0.00
------	------	------

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121515\
 Data File : BM003557.D
 Acq On : 15 Dec 2015 20:18
 Operator : UM/IZ
 Sample : PB87221BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 SBLK21

Manual Integrations
 APPROVED

MMdadoda
 12/16/2015 5:46:23 PM

Quant Time: Dec 16 06:12:53 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 16 05:49:57 2015
 Response via : Initial Calibration

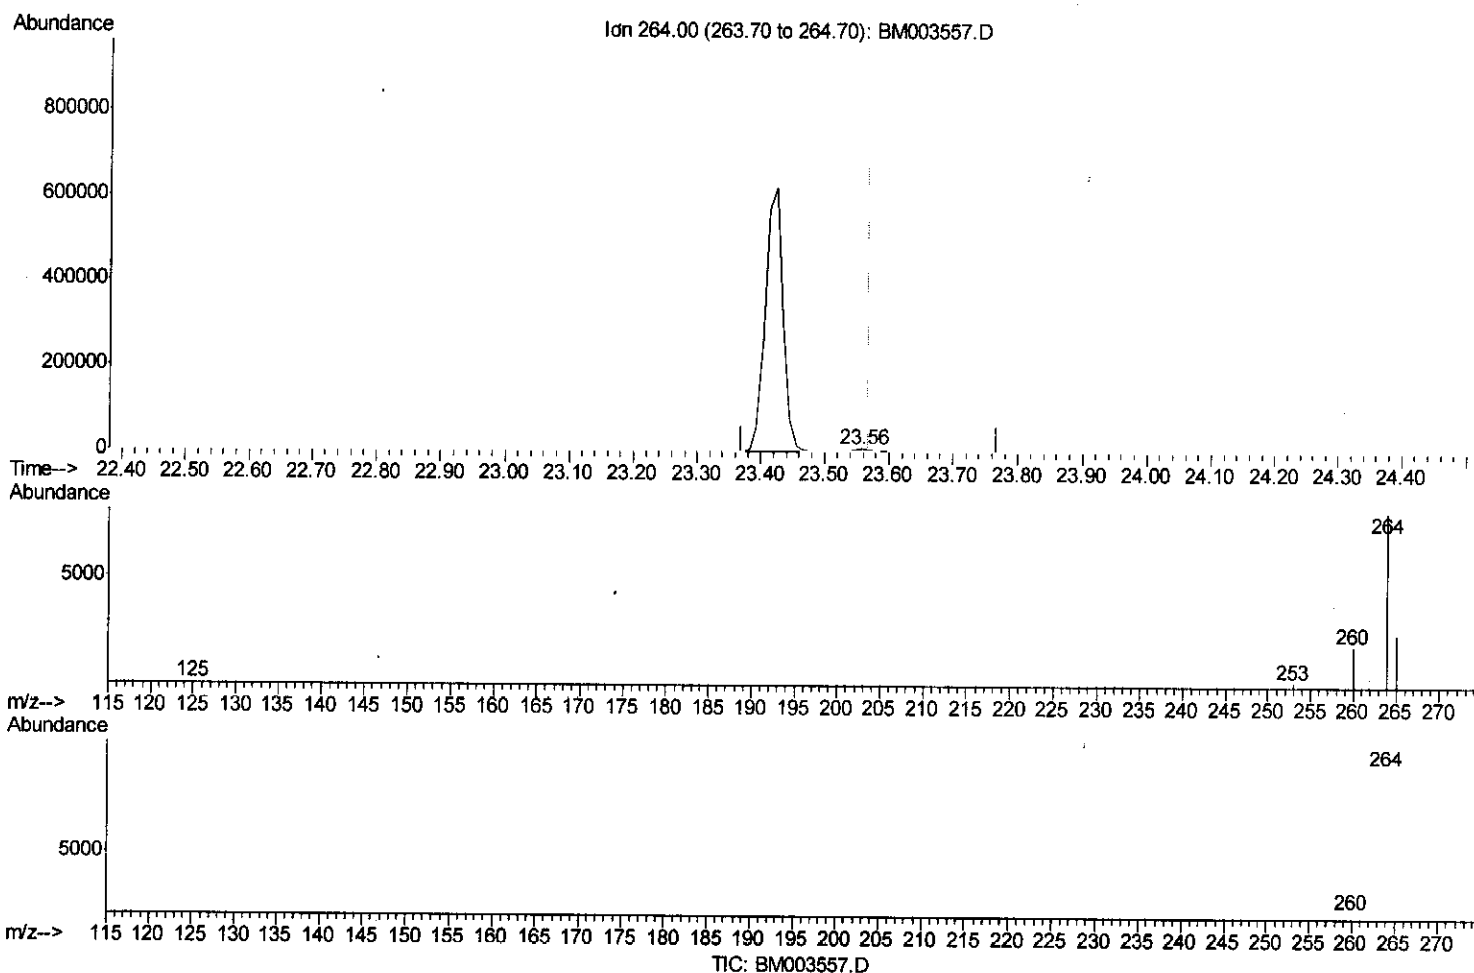

(22) Perylene-d12 (I)

23.559min (-0.010) 0.40ng/ul m

response 12522

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	25.40
265.00	38.20	32.18
0.00	0.00	0.00

U.M
 12/17/15

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM121515\
 Data File : BM003557.D
 Acq On : 15 Dec 2015 20:18
 Operator : UM/IZ
 Sample : FB87221BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK21

Manual Integrations
 APPROVED

MMdadoda
 12/16/2015 5:46:23 PM

Quant Time: Dec 16 06:27:29 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 16 05:49:57 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	4939	0.40	ng/ul	0.00
4) Naphthalene-d8	10.50	136	19442	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.37	164	10819	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.11	188	20874m	0.40	ng/ul	0.00
18) Chrysene-d12	21.31	240	18268	0.40	ng/ul	-0.01
22) Perylene-d12	23.56	264	12522m	0.40	ng/ul	-0.01
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.18	96	30435	14.42	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.10	152	8099	0.35	ng/ul	0.00
16) Fluoranthene-d10	19.15	212	14162	0.32	ng/ul	0.00

U.M
 12/17/15

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM121515\
 Data File : BM003557.D
 Acq On : 15 Dec 2015 20:18
 Operator : UM/IZ
 Sample : PB87221BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK21

Manual Integrations
 APPROVED

MMdadoda
 12/16/2015 5:46:23 PM

Quant Time: Dec 16 06:27:29 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 16 05:49:57 2015
 Response via : Initial Calibration

