

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121515\
 Data File : BM003559.D
 Acq On : 15 Dec 2015 21:30
 Operator : UM/IZ
 Sample : G4734-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4KW1

Manual Integrations
 APPROVED

MMdadoda
 12/16/2015 6:38:58 PM

Quant Time: Dec 16 17:31:16 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 16 05:49:57 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	4975	0.40	ng/ul	0.00
4) Naphthalene-d8	10.50	136	20625	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.37	164	12454	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.11	188	27109m	0.40	ng/ul	0.00
18) Chrysene-d12	21.31	240	27726	0.40	ng/ul	0.00
22) Perylene-d12	23.57	264	20407m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
6) 2-Methylnaphthalene-d10	12.10	152	9404	0.38	ng/ul	0.00
16) Fluoranthene-d10	19.14	212	23004	0.40	ng/ul	0.00
Target Compounds						
21) Chrysene	21.35	228	2417	0.03	ng/ul#	Ovalue 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM121515\
Data File : BM003559.D
Acq On : 15 Dec 2015 21:30
Operator : UM/IZ
Sample : G4734-01
Misc :
ALS Vial : 9 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A4KW1

Manual Integrations
APPROVED

MMdadoda
12/16/2015 6:38:58 PM

Quant Time: Dec 16 17:31:16 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM121515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 16 05:49:57 2015
Response via : Initial Calibration

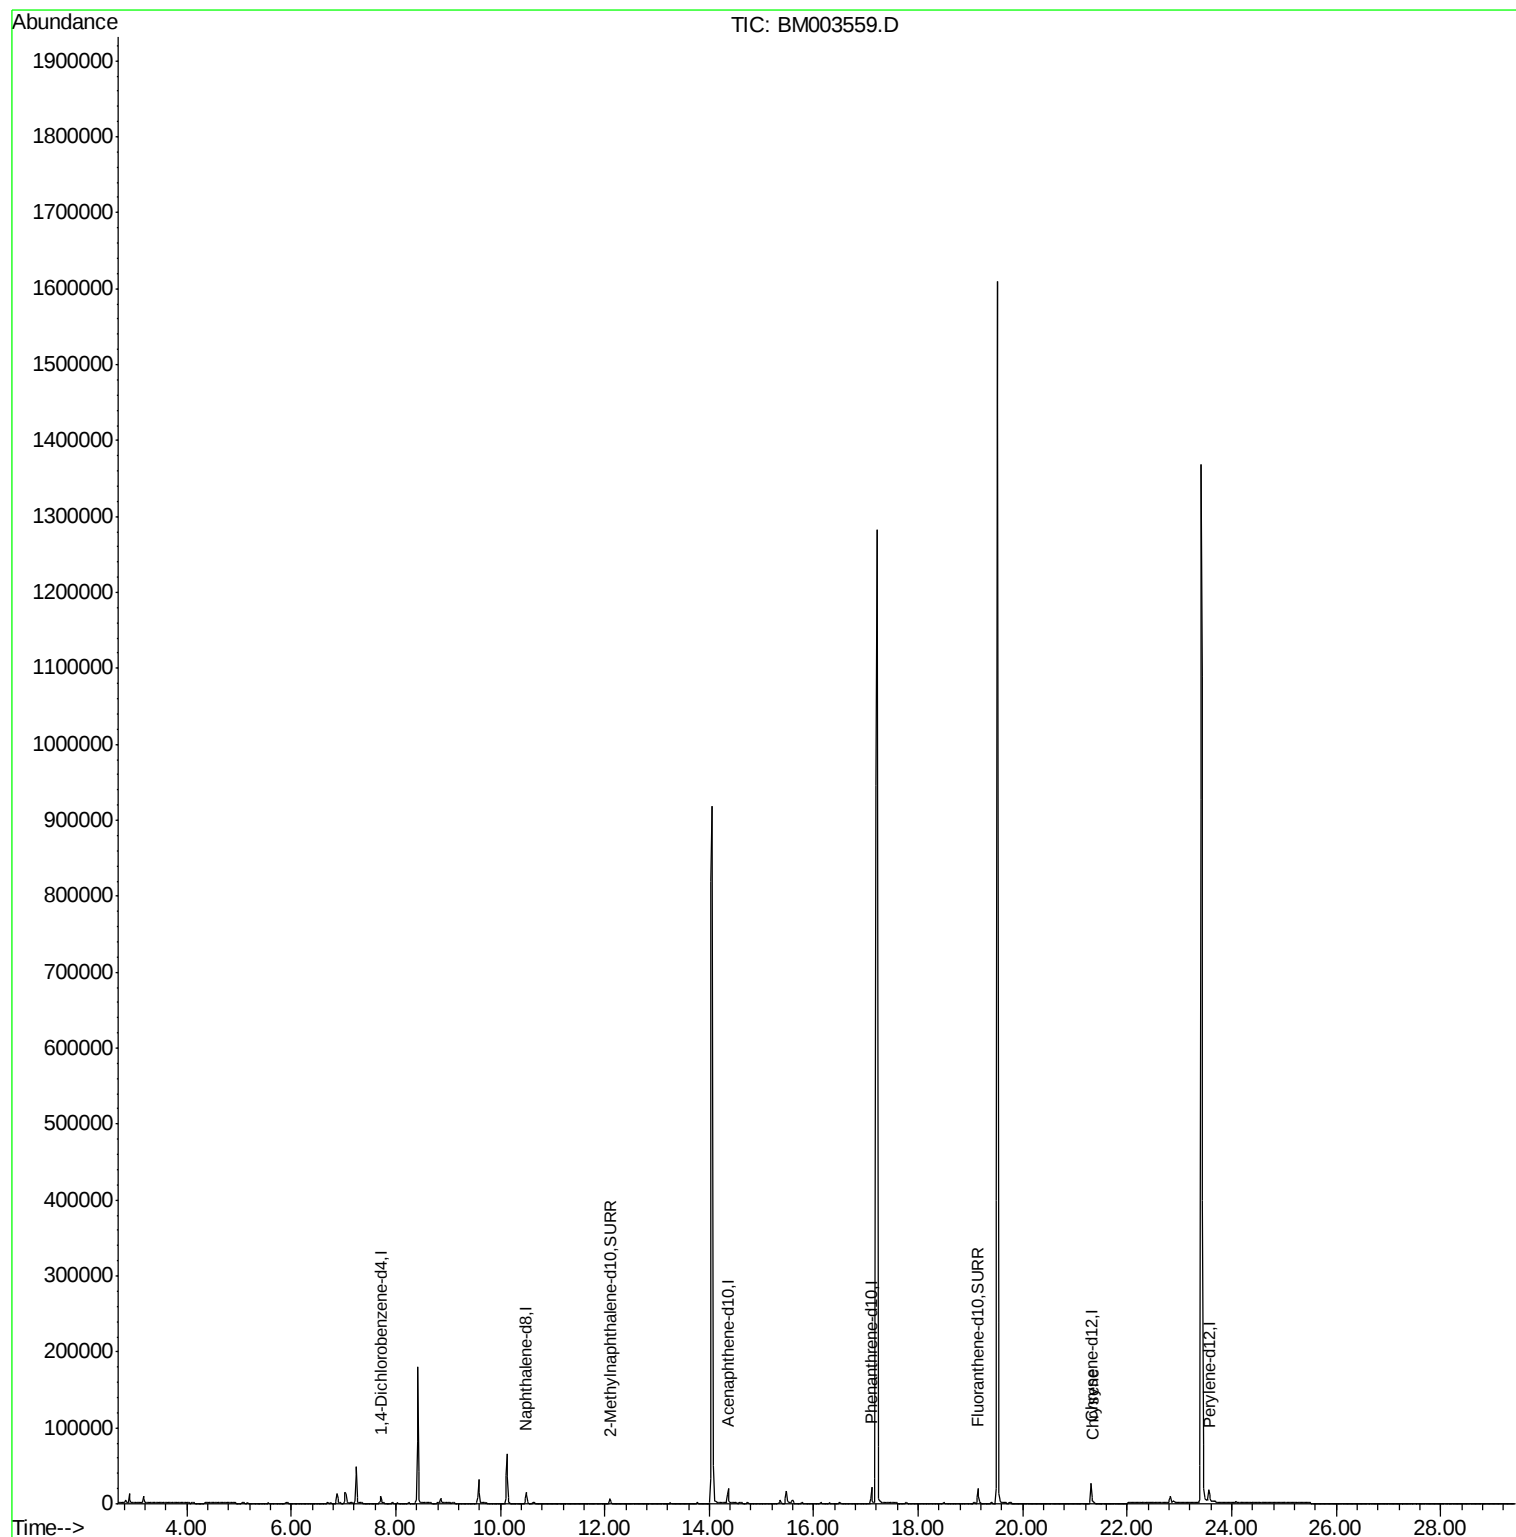

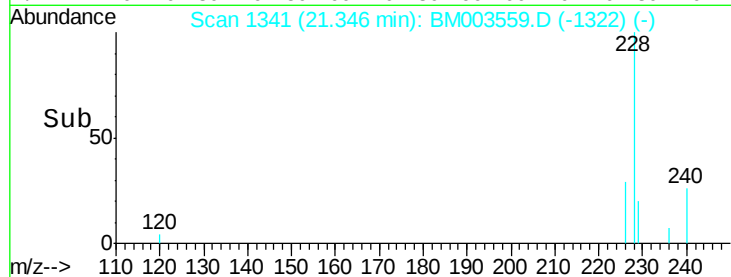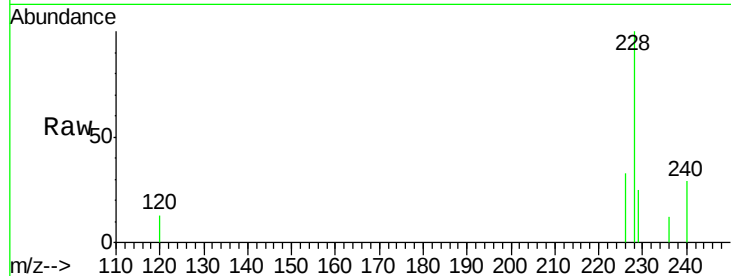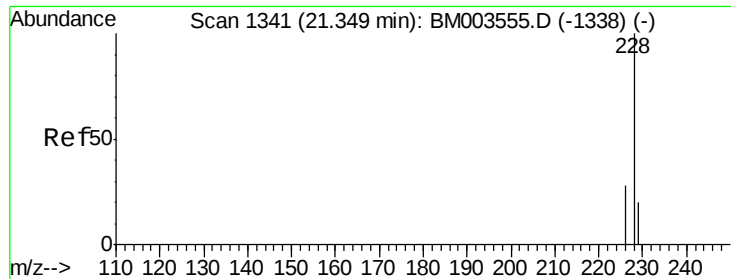

#21

Chrysene

Concen: 0.03 ng/ul

RT: 21.35 min Scan# 1341

Delta R.T. -0.00 min

Lab File: BM003559.D

Acq: 15 Dec 2015 21:30

Tot Ion:	228	Resp:	2417
Ion Ratio	Lower	Upper	
228	100		
226	32.7	21.2	31.8#
229	24.7	17.0	25.6

Instrument :

BNA_M

ClientSampleId :

A4KW1

Manual Integrations
APPROVED

MMdadoda
12/16/2015 6:38:58 PM

