
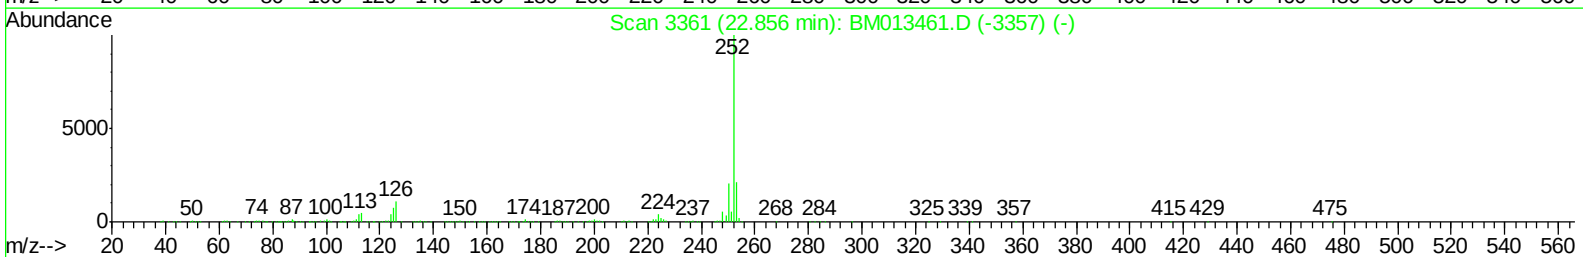
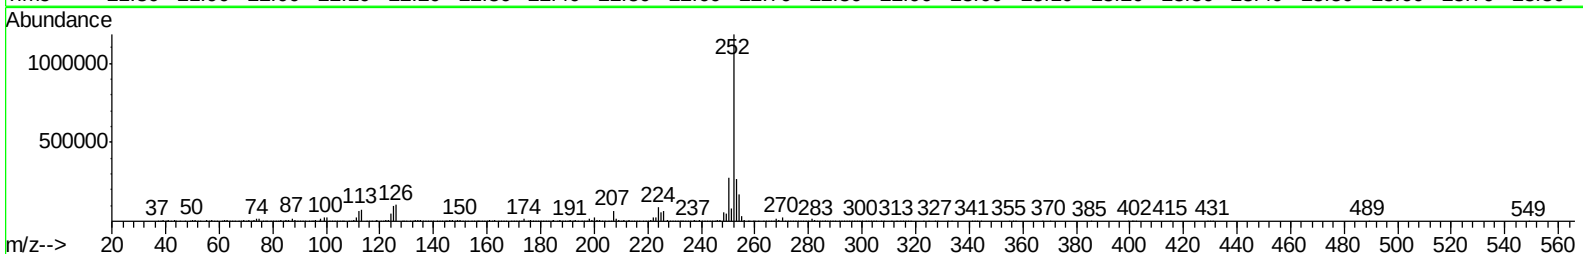


Data File : BM013463.D
Acq On : 16 Dec 2017 05:51
Operator : SJ/JU
Sample : I6801-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Dec 18 00:27:19 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

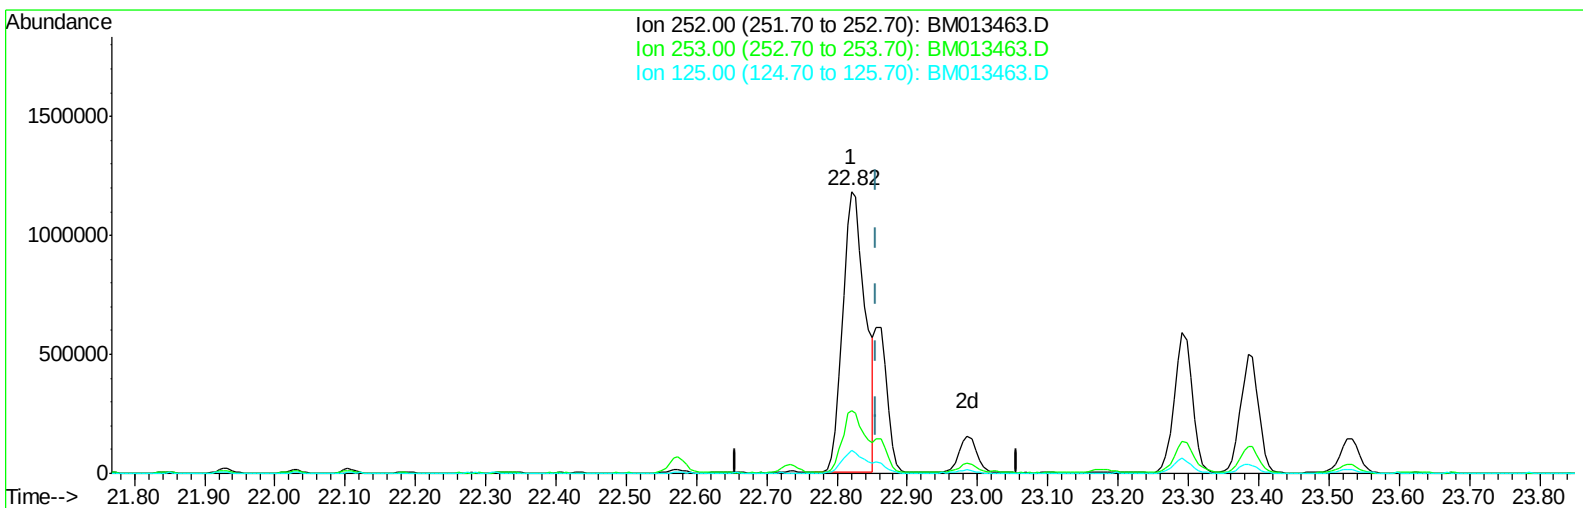

TIC: BM013463.D

(86) Benzo(k)fluoranthene

22.821min (-0.036) 42.47ng/ul

response 2675168

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.48
125.00	4.30	8.14#
0.00	0.00	0.00