
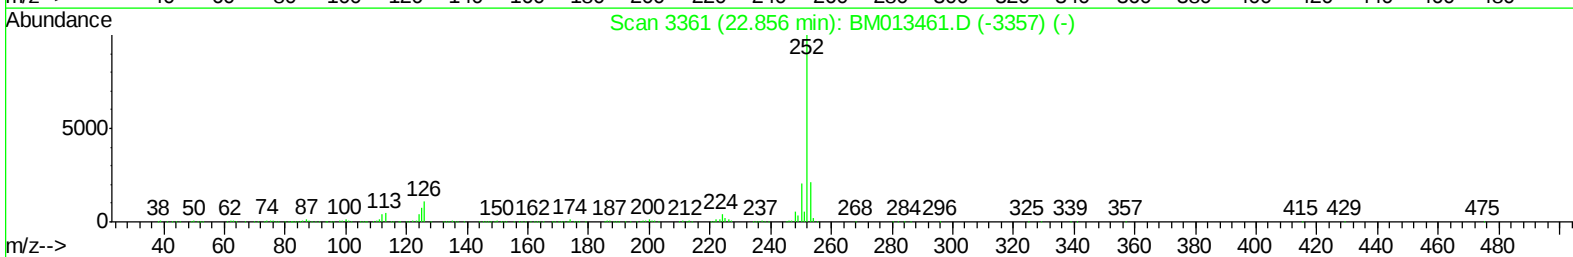
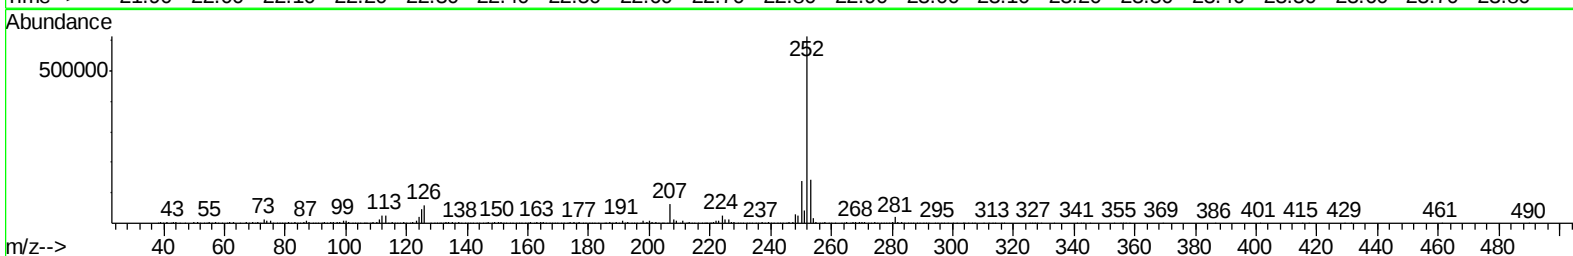


Data File : BM013463.D
Acq On : 16 Dec 2017 05:51
Operator : SJ/JU
Sample : I6801-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Dec 18 00:27:19 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

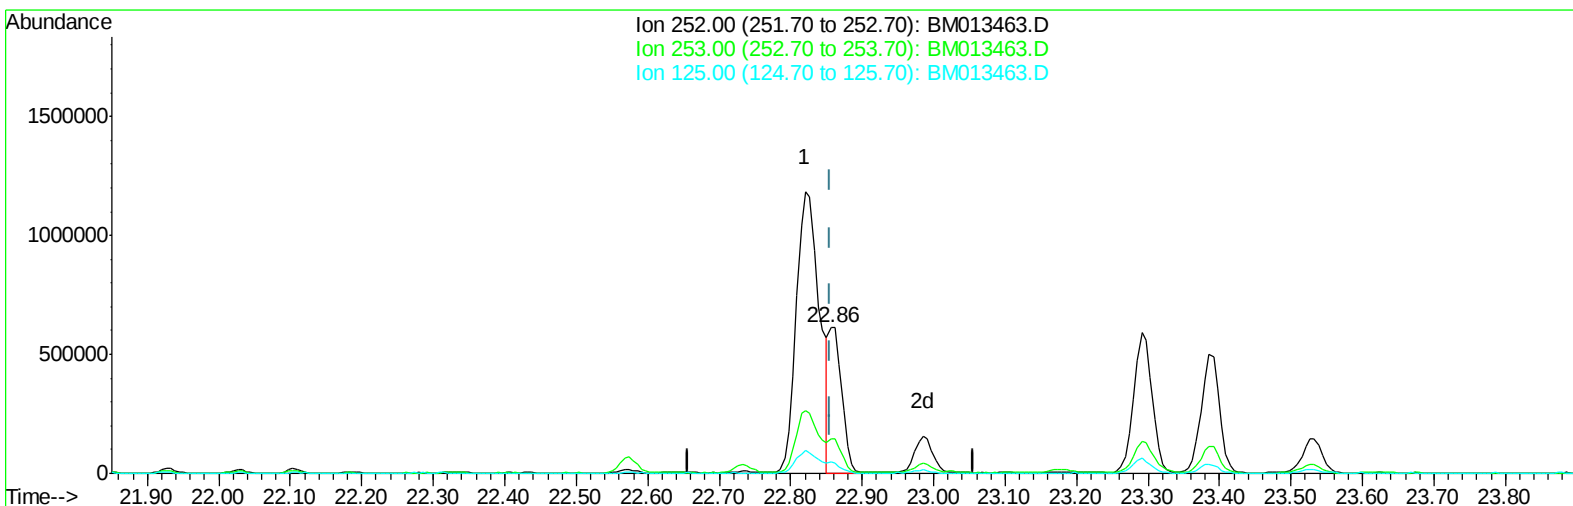

TIC: BM013463.D

(86) Benzo(k)fluoranthene

22.856min (-0.000) 11.84ng/ul m

response 745998

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	23.35
125.00	4.30	7.82#
0.00	0.00	0.00