
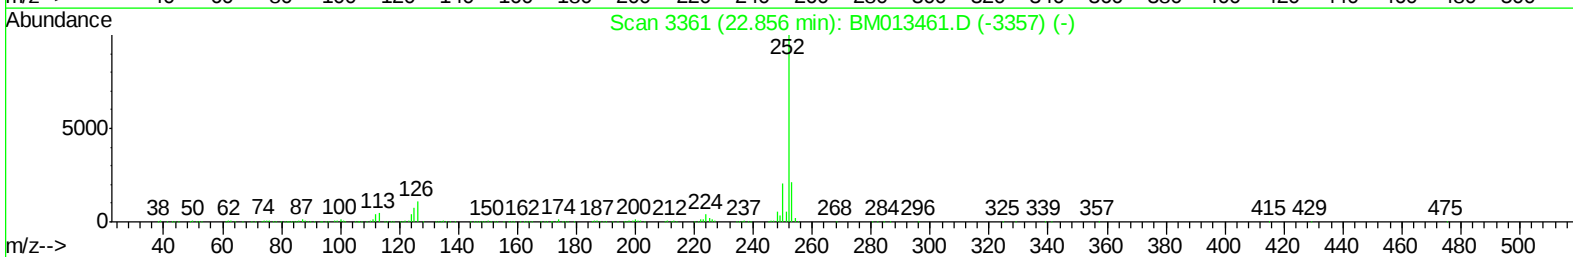
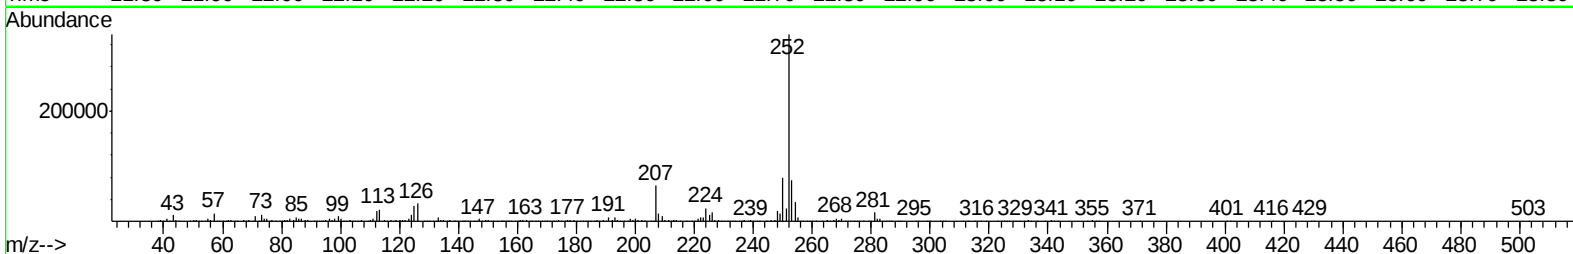


Data File : BM013464.D
Acq On : 16 Dec 2017 06:26
Operator : SJ/JU
Sample : I6775-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Dec 18 00:27:37 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

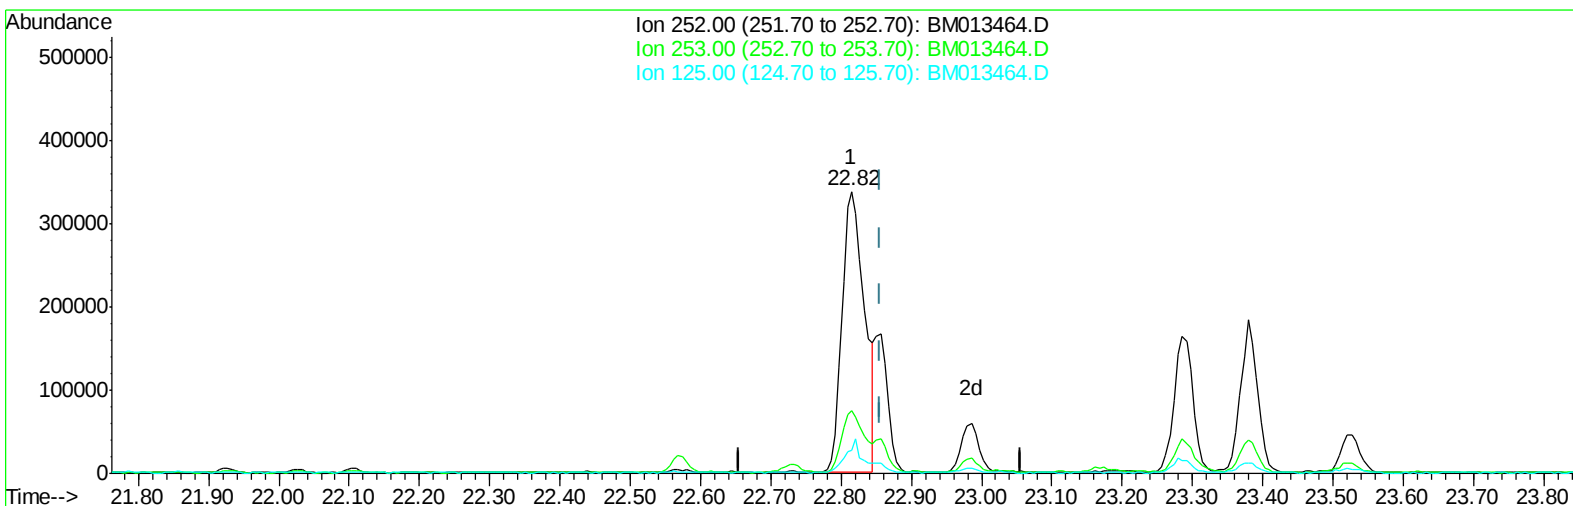

TIC: BM013464.D

(86) Benzo(k)fluoranthene

22.815min (-0.041) 12.46ng/ul

response 759729

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.26
125.00	4.30	8.06#
0.00	0.00	0.00