
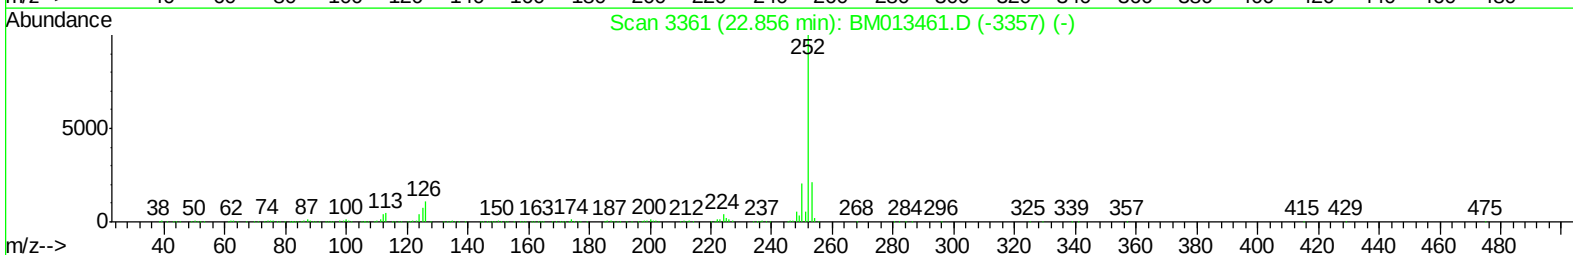
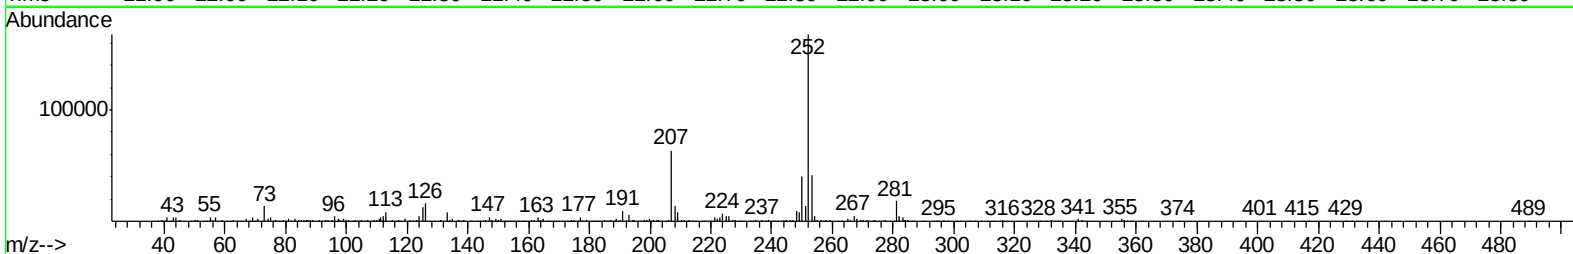


Data File : BM013464.D
Acq On : 16 Dec 2017 06:26
Operator : SJ/JU
Sample : I6775-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Dec 18 00:27:37 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

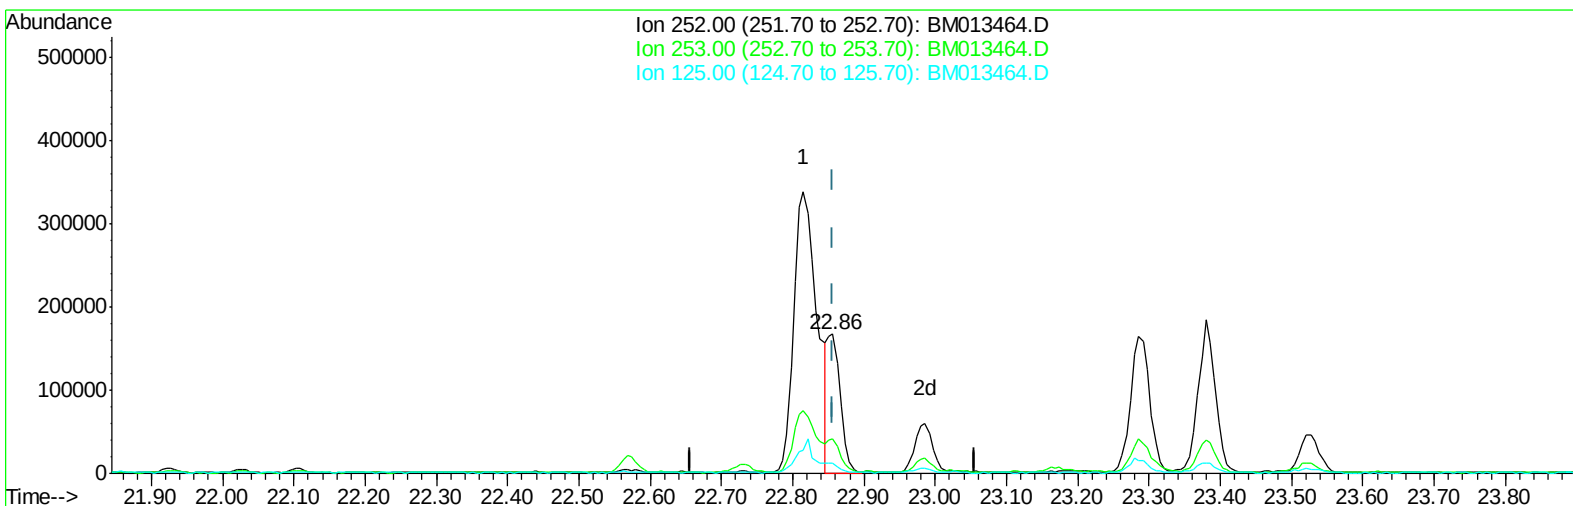

TIC: BM013464.D

(86) Benzo(k)fluoranthene

22.856min (-0.000) 3.48ng/ul m

response 212520

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	24.86
125.00	4.30	7.47#
0.00	0.00	0.00