
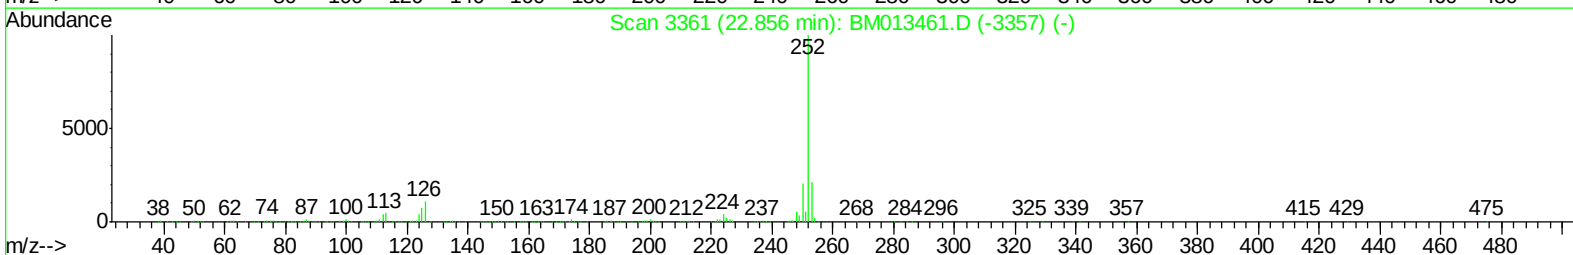
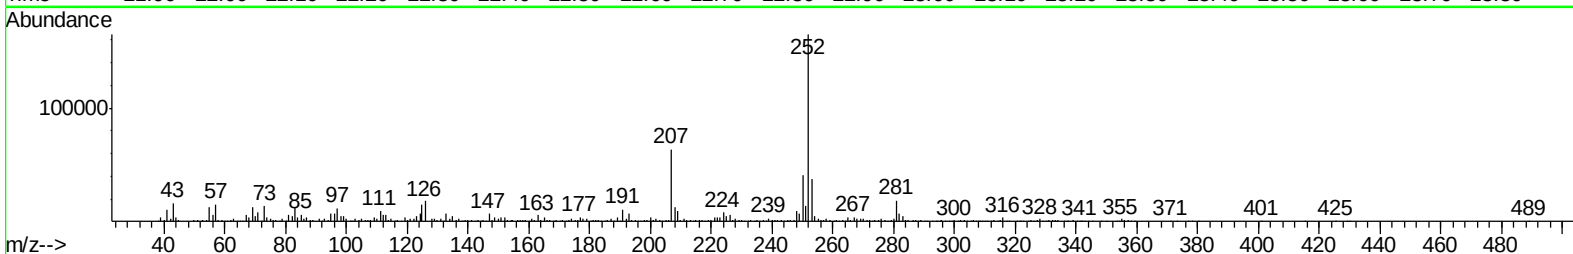


Data File : BM013466.D
Acq On : 16 Dec 2017 07:37
Operator : SJ/JU
Sample : I6776-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Dec 18 01:02:19 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

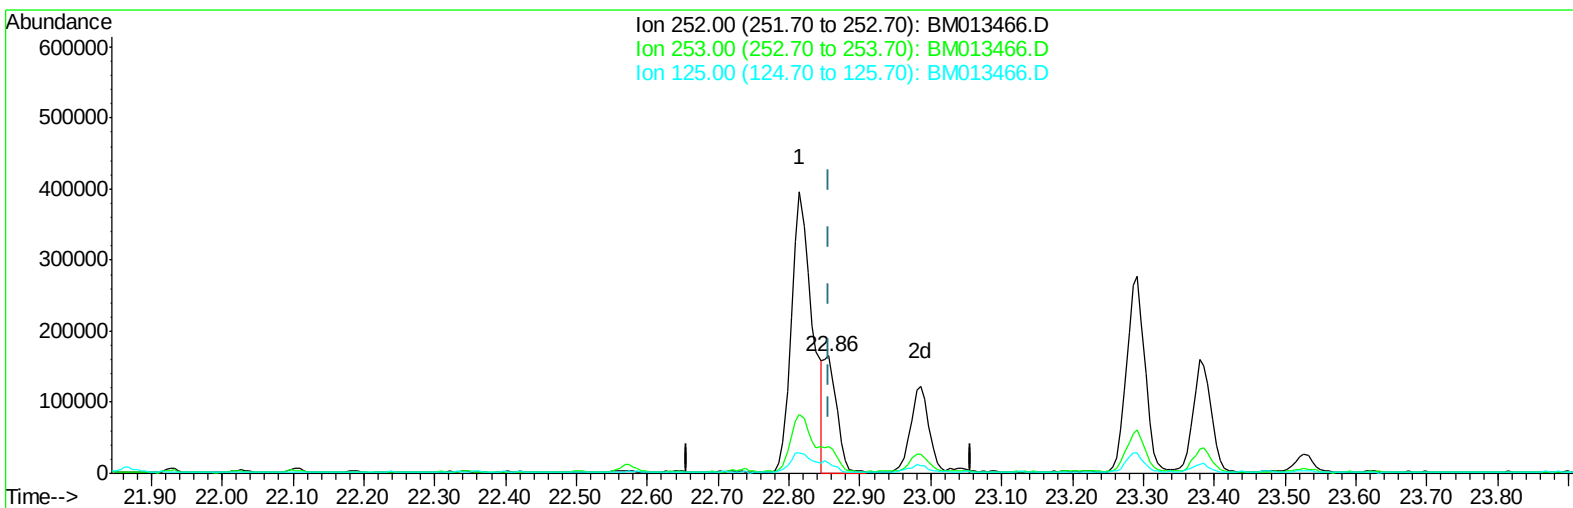

TIC: BM013466.D

(86) Benzo(k)fluoranthene

22.856min (-0.000) 3.11ng/ul m

response 220752

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.52
125.00	4.30	8.82#
0.00	0.00	0.00