
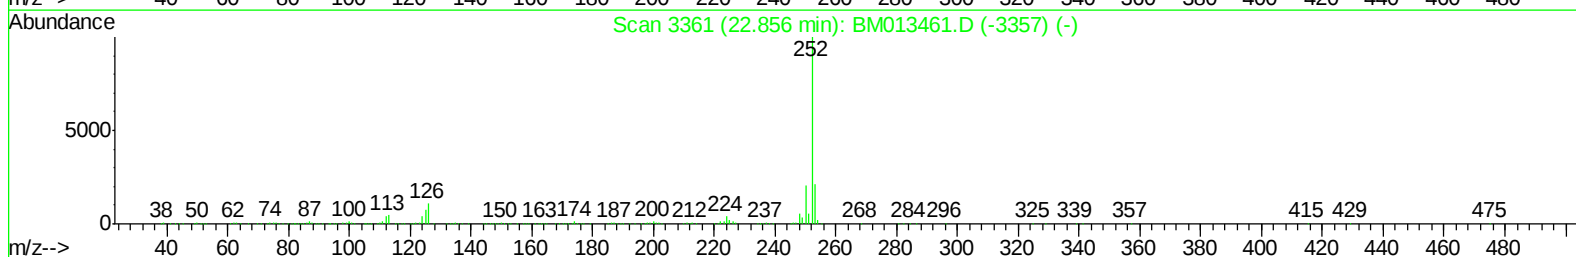
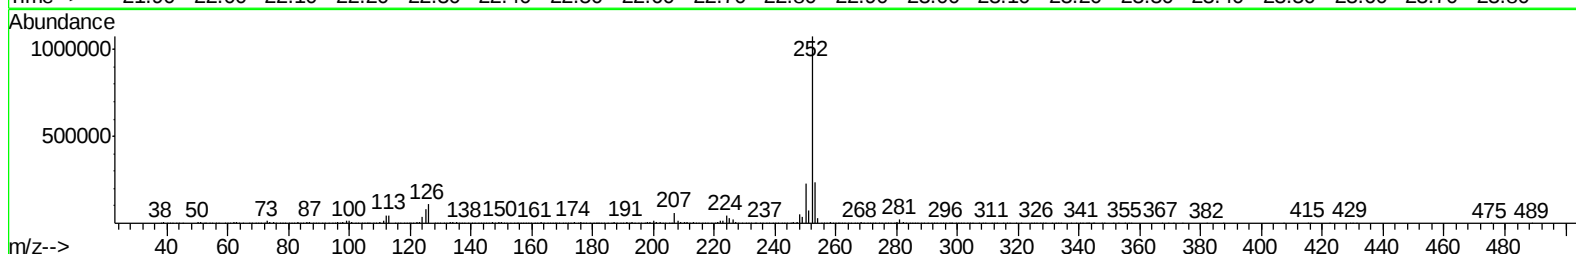


Data File : BM013467.D
Acq On : 16 Dec 2017 08:13
Operator : SJ/JU
Sample : I6776-06 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Dec 18 00:28:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

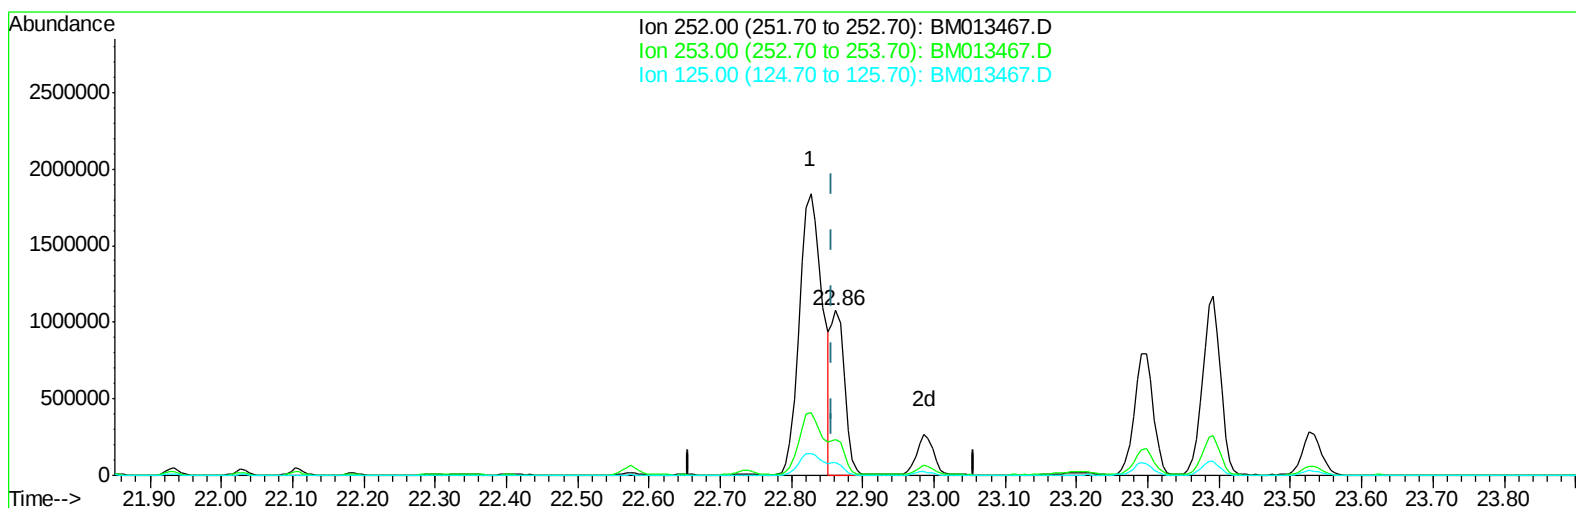

TIC: BM013467.D

(86) Benzo(k)fluoranthene

22.862min (+0.006) 24.78ng/ul m

response 1462470

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.12
125.00	4.30	7.66#
0.00	0.00	0.00