
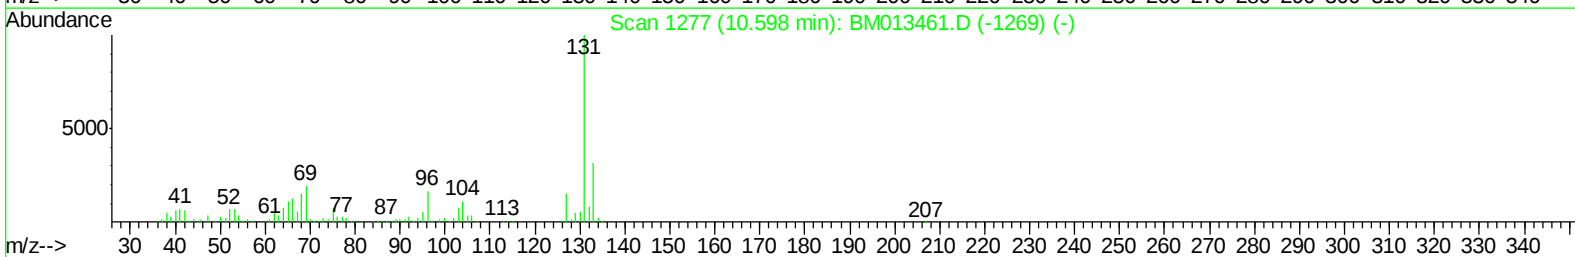
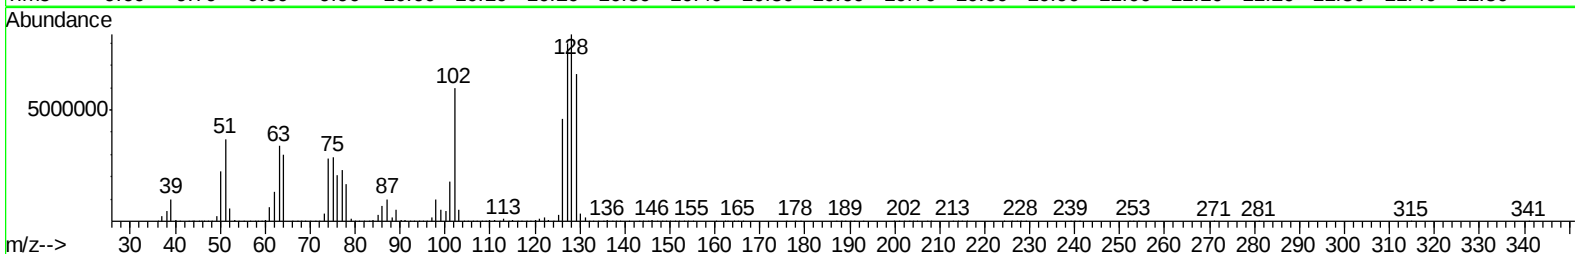


Data File : BM013468.D
Acq On : 16 Dec 2017 08:48
Operator : SJ/JU
Sample : I6775-07 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Dec 18 00:28:55 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

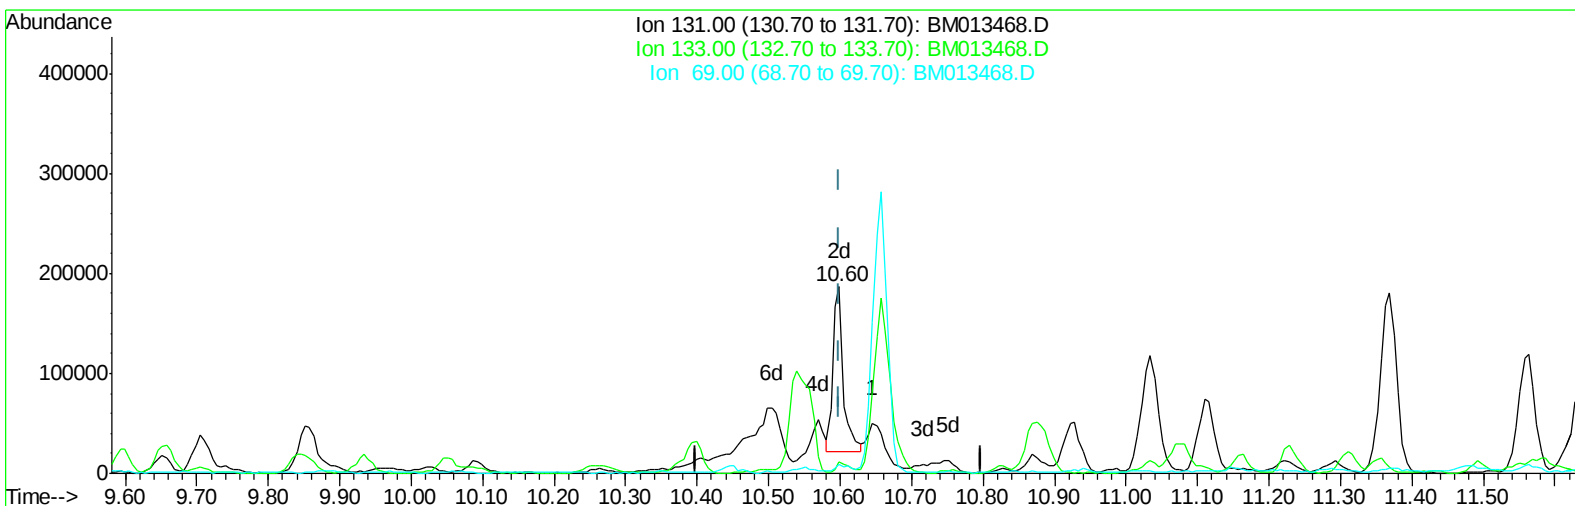

TIC: BM013468.D

(29) 4-Chloroaniline-d4 (S)

10.599min (+0.000) 8.64ng/ul m

response 163812

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	5.98#
69.00	24.30	4.50#
0.00	0.00	0.00