
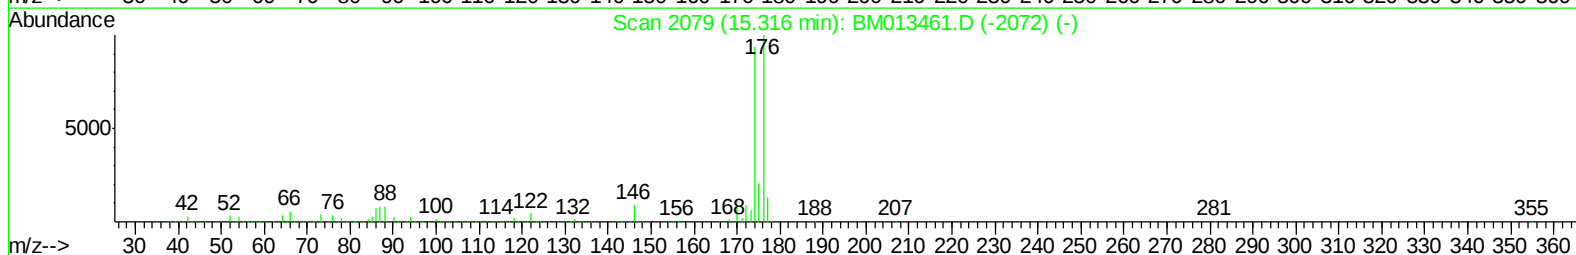
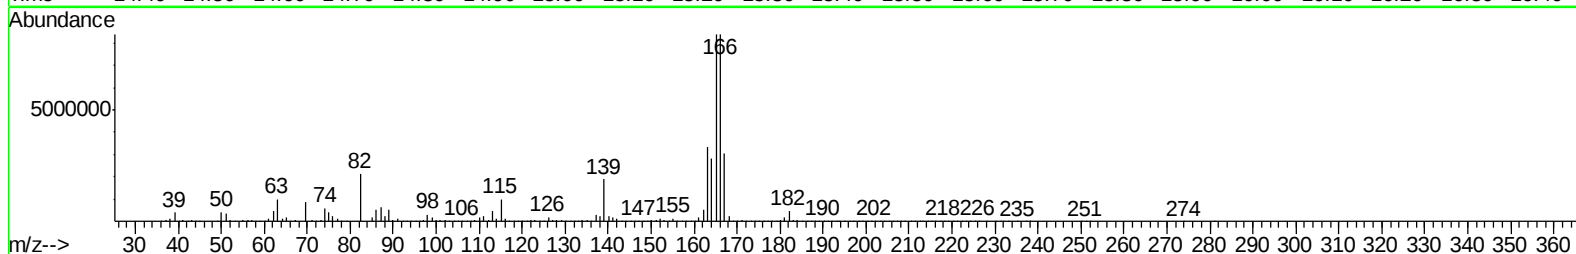


Data File : BM013468.D
Acq On : 16 Dec 2017 08:48
Operator : SJ/JU
Sample : I6775-07 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Dec 18 01:25:12 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

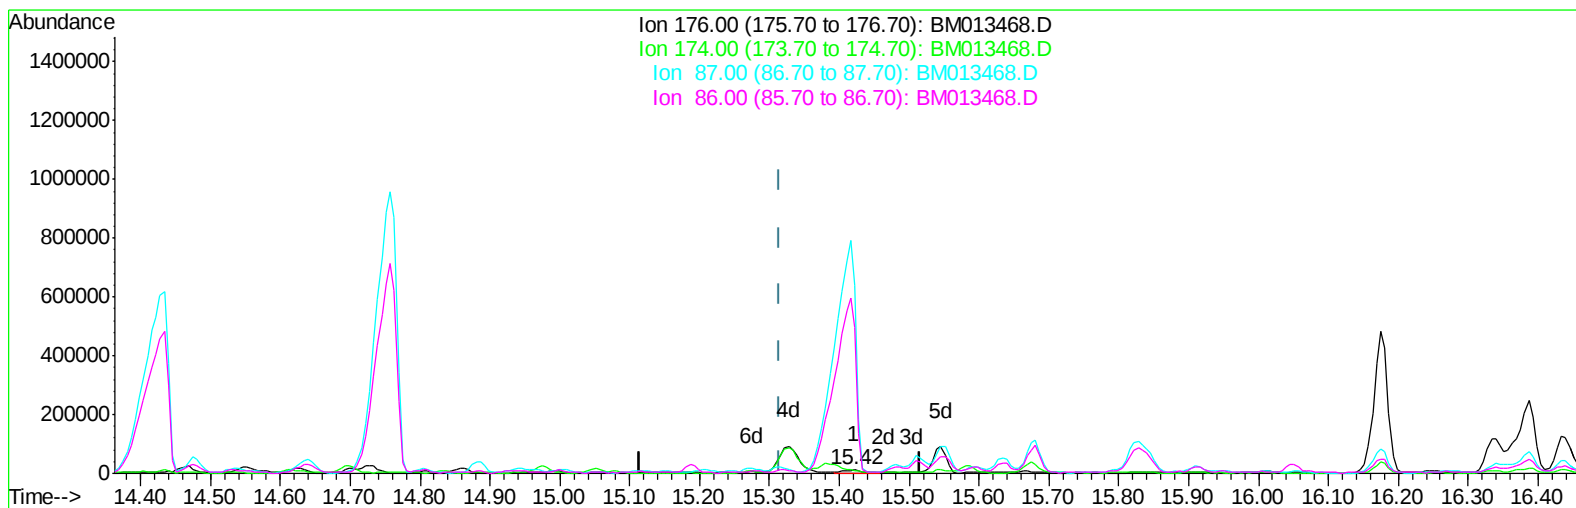

TIC: BM013468.D

(57) Fluorene-d10 (S)

15.422min (+0.106) 0.27ng/ul

response 14765

Ion	Exp%	Act%
176.00	100	100
174.00	95.20	78.93
87.00	6.30	5609.07#
86.00	5.90	4366.99#