
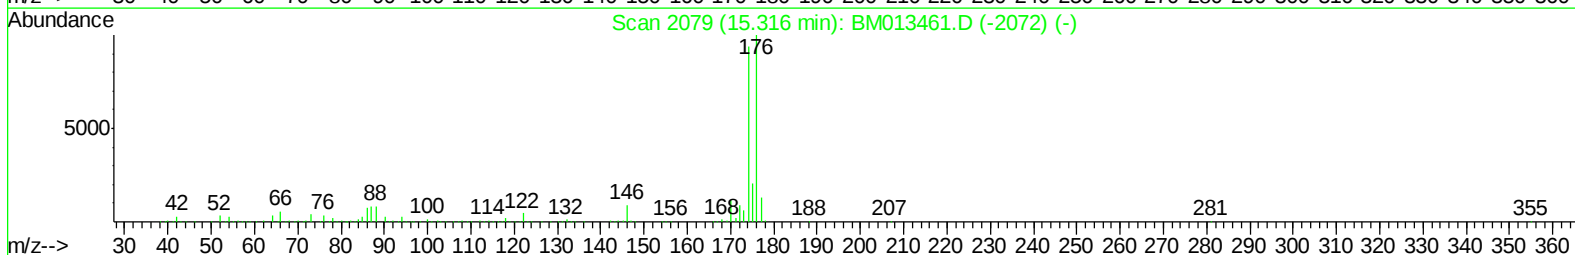
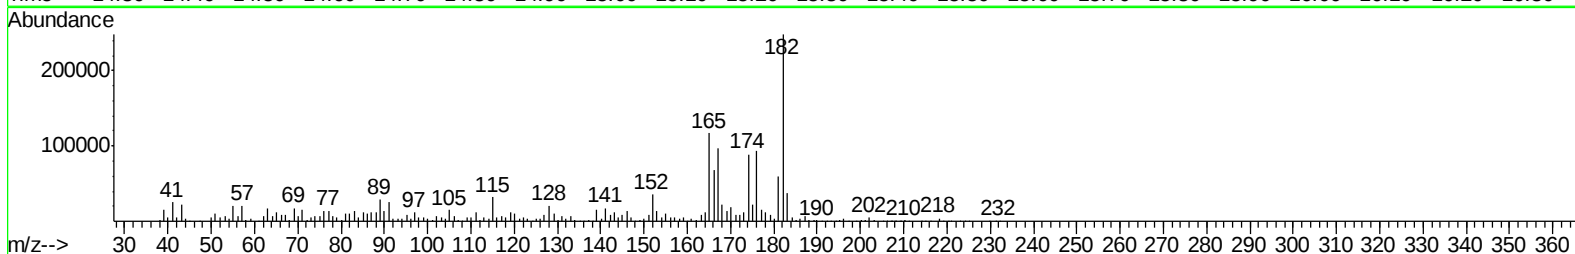


Data File : BM013468.D
Acq On : 16 Dec 2017 08:48
Operator : SJ/JU
Sample : I6775-07 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Dec 18 01:25:12 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

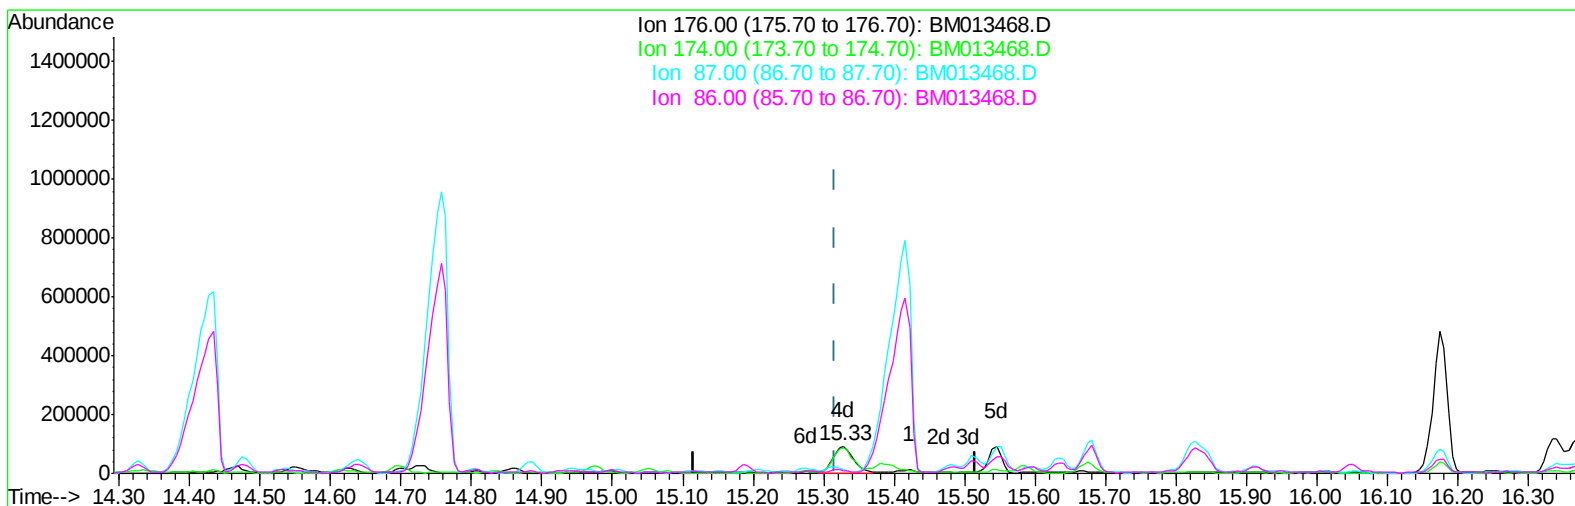

TIC: BM013468.D

(57) Fluorene-d10 (S)

15.328min (+0.012) 3.43ng/ul m

response 188515

Ion	Exp%	Act%
176.00	100	100
174.00	95.20	95.50
87.00	6.30	13.84#
86.00	5.90	10.64#