
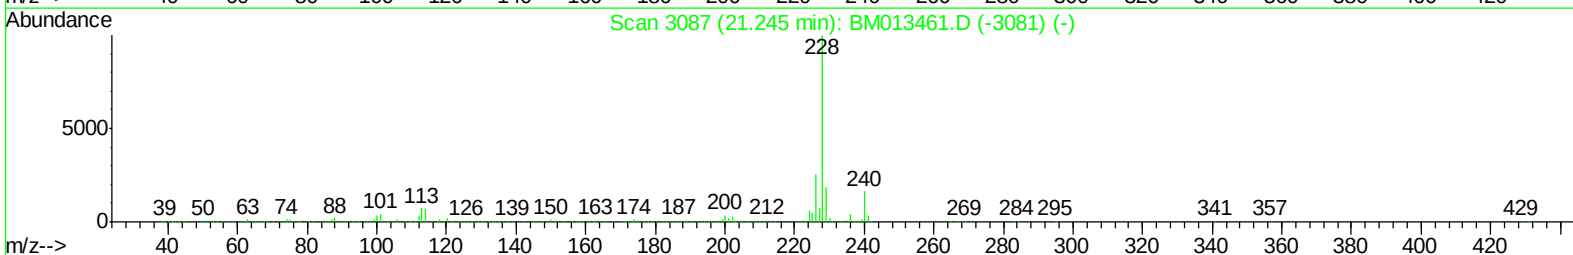
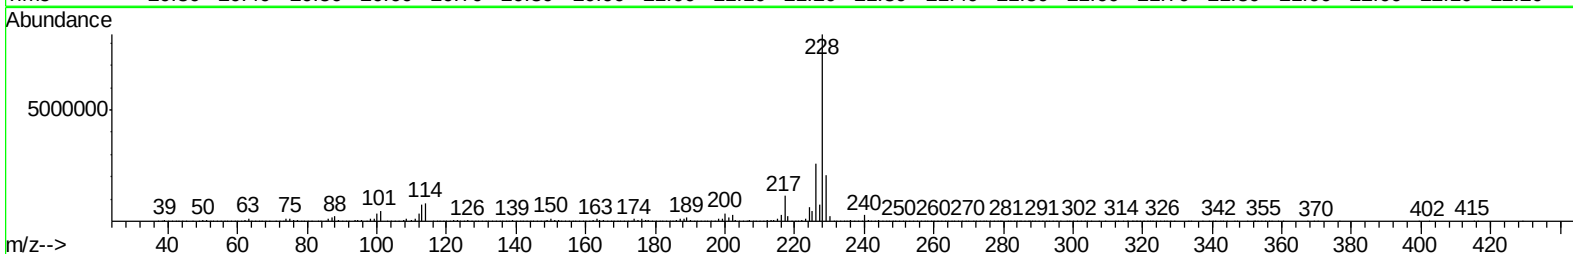


Data File : BM013468.D
Acq On : 16 Dec 2017 08:48
Operator : SJ/JU
Sample : I6775-07 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Dec 18 01:25:12 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

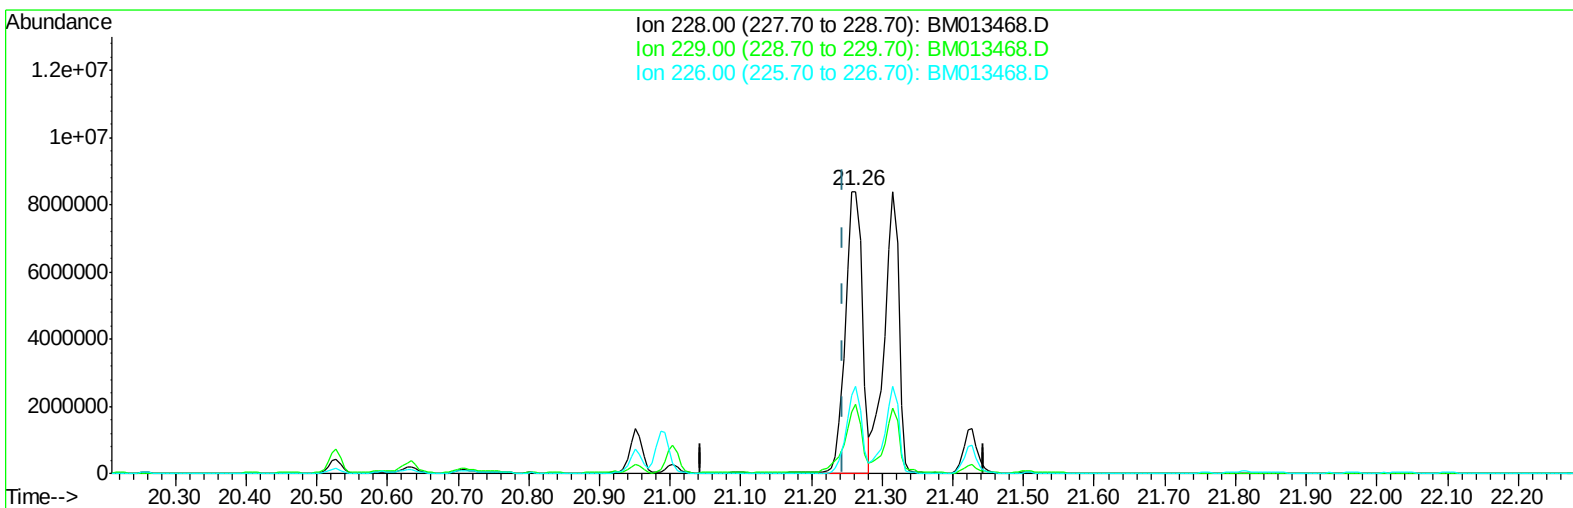

TIC: BM013468.D

(80) Benzo(a)anthracene
21.263min (+0.018) 206.94ng/ul m
response 13818785

Ion	Exp%	Act%
228.00	100	100
229.00	19.20	24.44#
226.00	26.70	31.13
0.00	0.00	0.00