
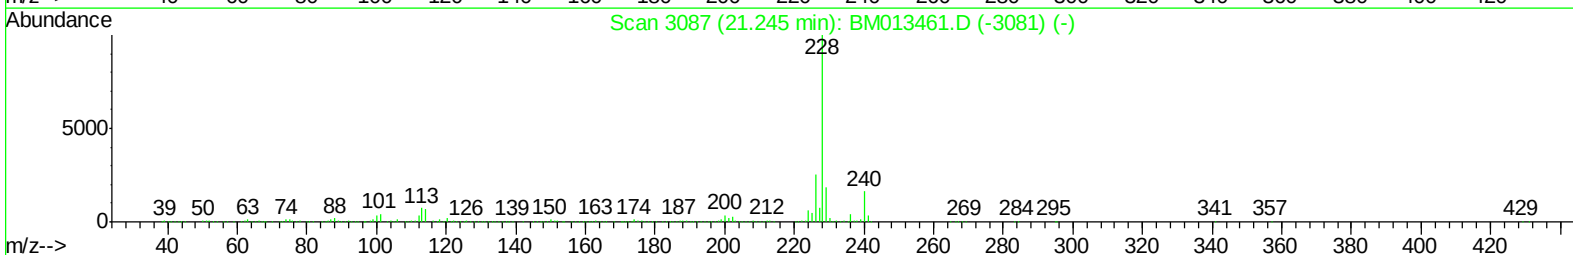
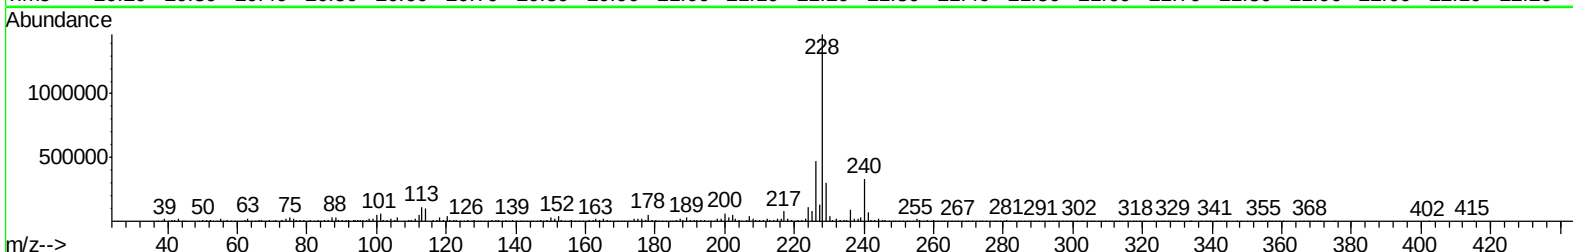


Data File : BM013470.D
Acq On : 16 Dec 2017 09:59
Operator : SJ/JU
Sample : I6776-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Dec 18 00:29:47 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

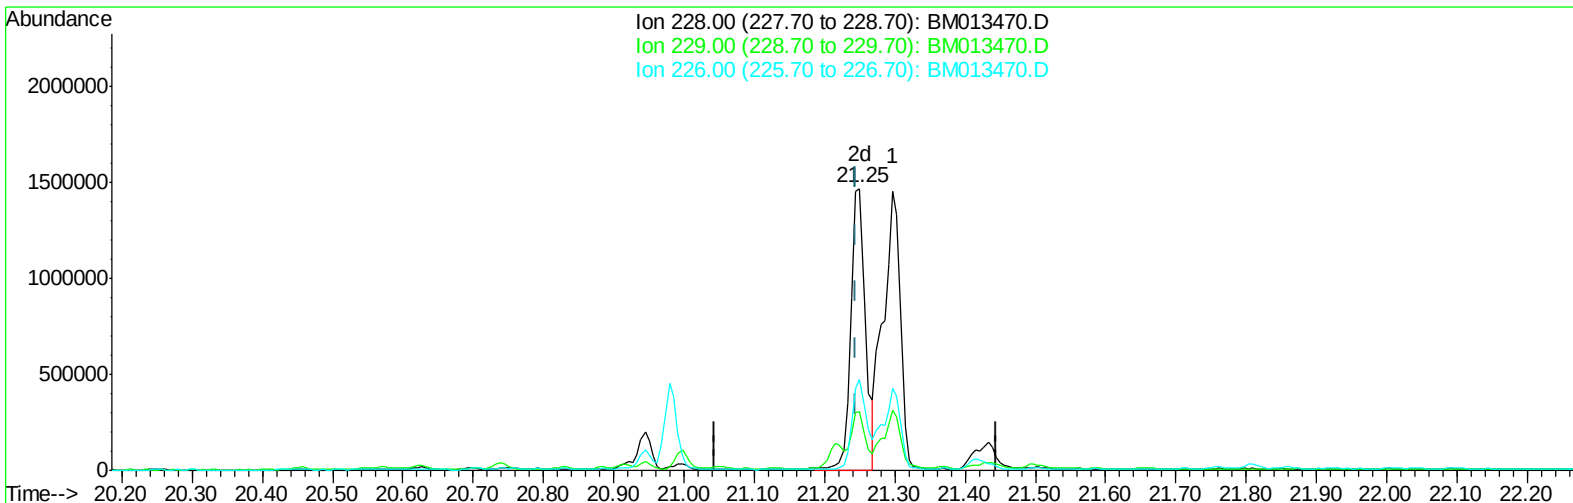

TIC: BM013470.D

(80) Benzo(a)anthracene

21.250min (+0.006) 26.88ng/ul m

response 2144004

Ion	Exp%	Act%
228.00	100	100
229.00	19.20	20.80
226.00	26.70	32.27#
0.00	0.00	0.00