
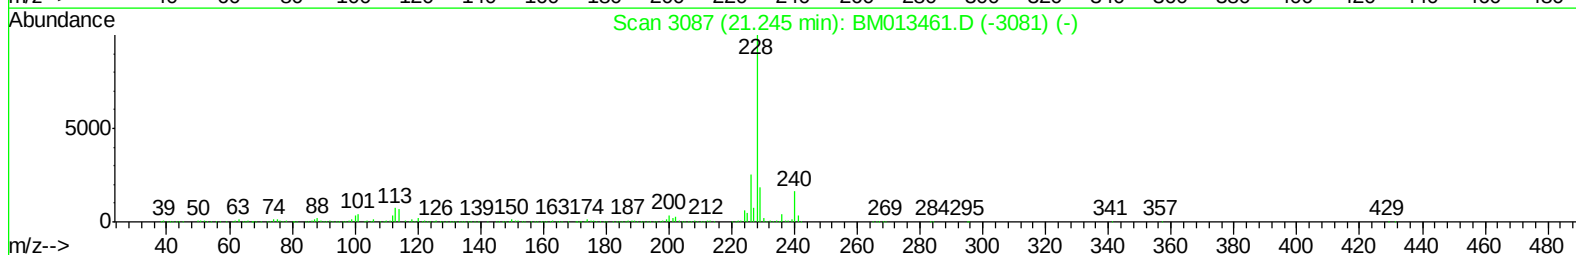
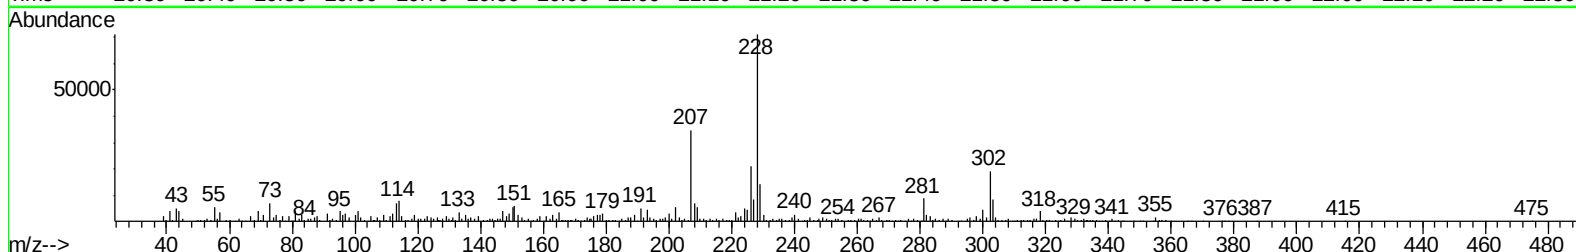


Data File : BM013471.D
Acq On : 16 Dec 2017 10:35
Operator : SJ/JU
Sample : I6799-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Dec 18 00:30:05 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

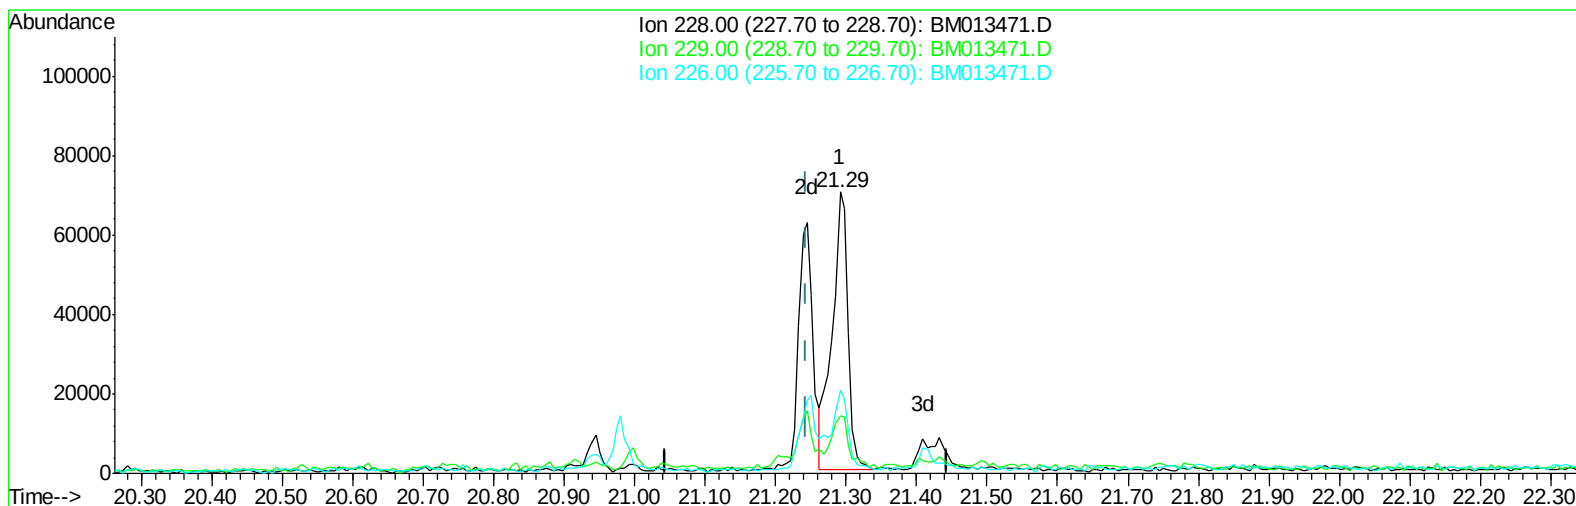

TIC: BM013471.D

(80) Benzo(a)anthracene
21.291min (+0.047) 1.27ng/ul

response 107856

Ion	Exp%	Act%
228.00	100	100
229.00	19.20	20.38
226.00	26.70	29.48
0.00	0.00	0.00