
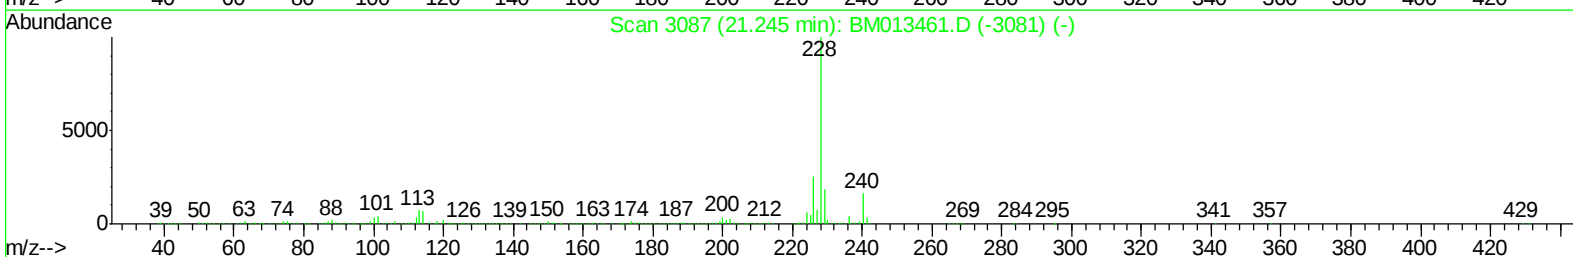
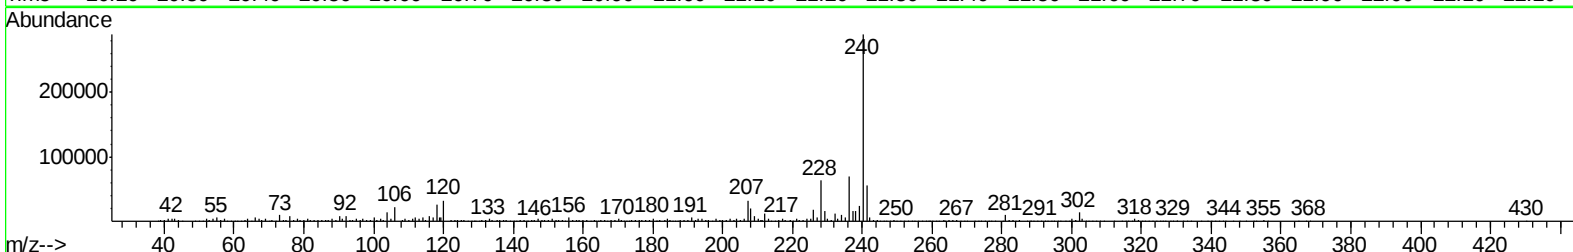


Data File : BM013471.D
Acq On : 16 Dec 2017 10:35
Operator : SJ/JU
Sample : I6799-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Dec 18 00:30:05 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

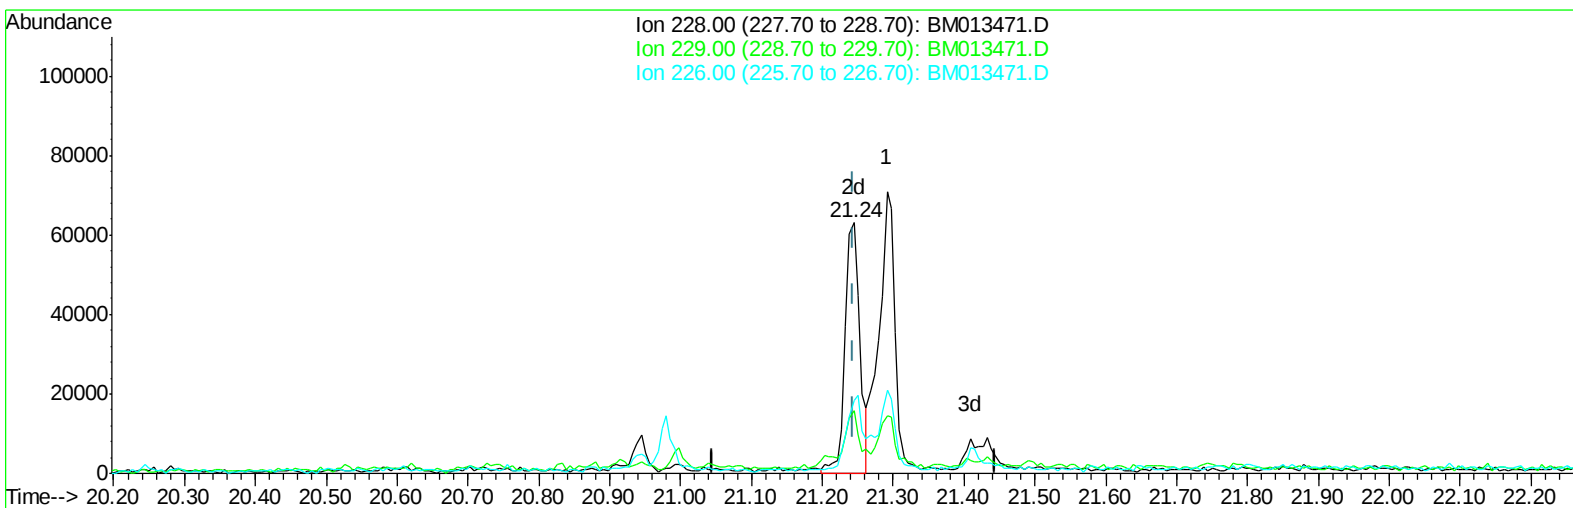

TIC: BM013471.D

(80) Benzo(a)anthracene

21.244min (-0.000) 1.09ng/ul m

response 92644

Ion	Exp%	Act%
228.00	100	100
229.00	19.20	25.03#
226.00	26.70	28.88
0.00	0.00	0.00