
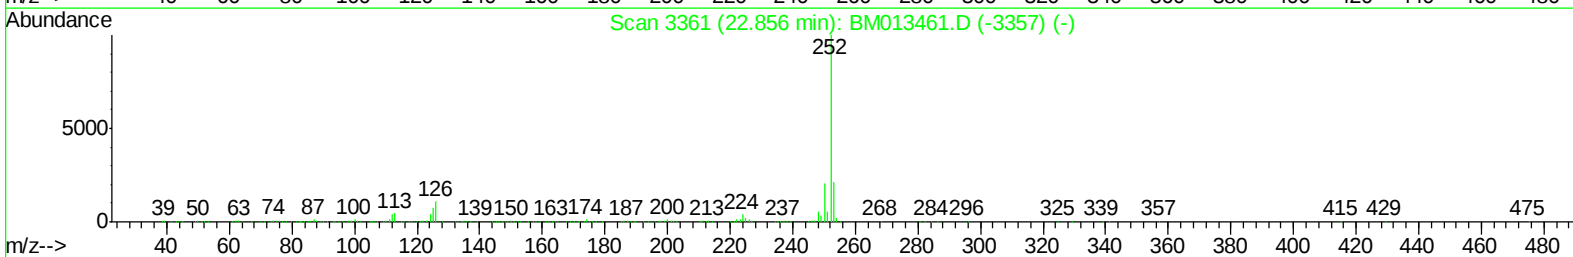
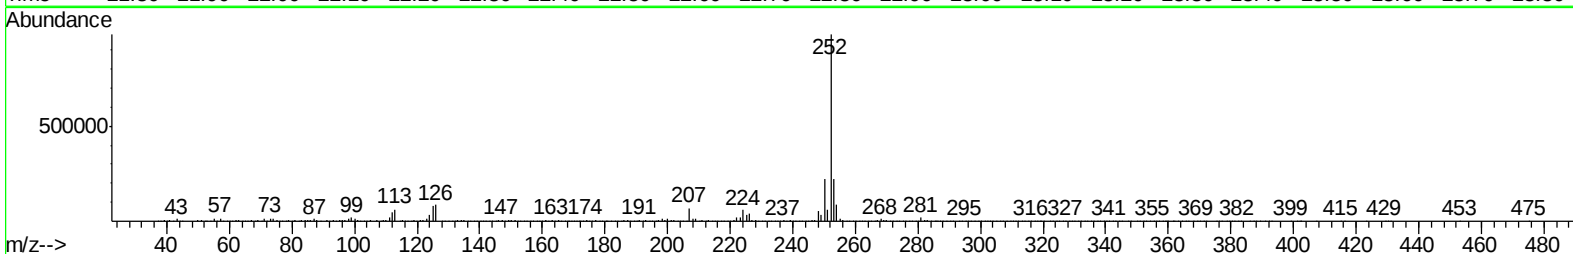


Data File : BM013473.D
Acq On : 16 Dec 2017 11:46
Operator : SJ/JU
Sample : I6778-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Dec 18 00:30:38 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

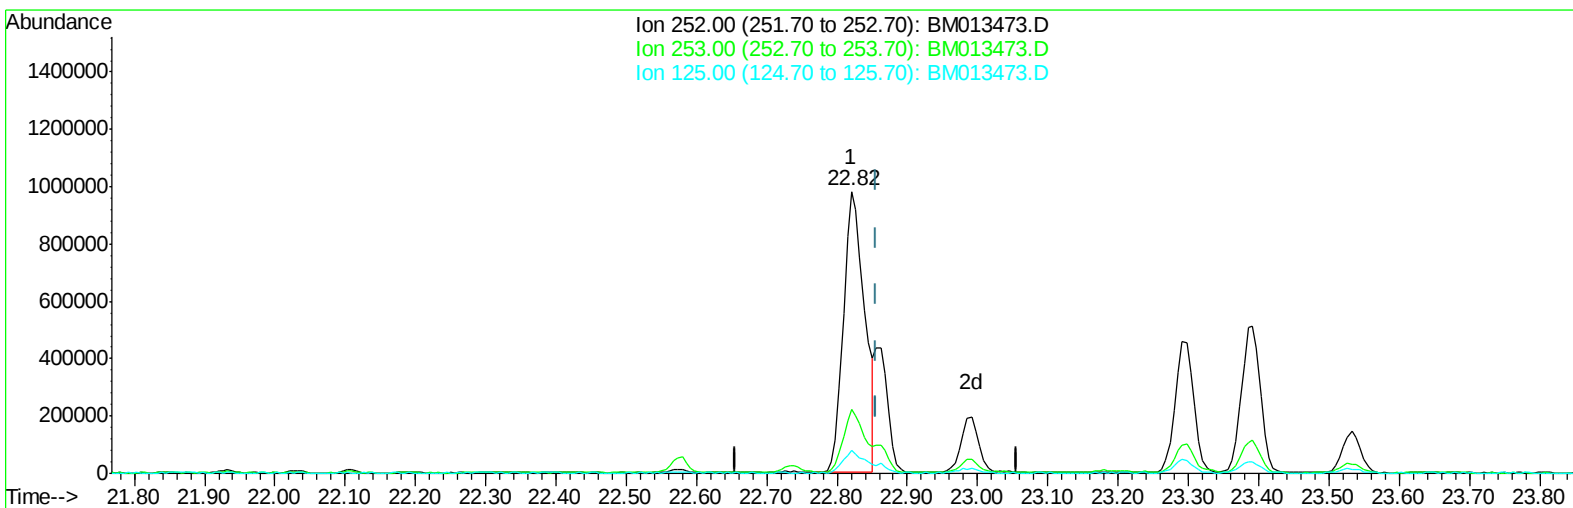

TIC: BM013473.D

(86) Benzo(k)fluoranthene

22.821min (-0.036) 29.45ng/ul

response 2079680

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.52
125.00	4.30	8.22#
0.00	0.00	0.00