
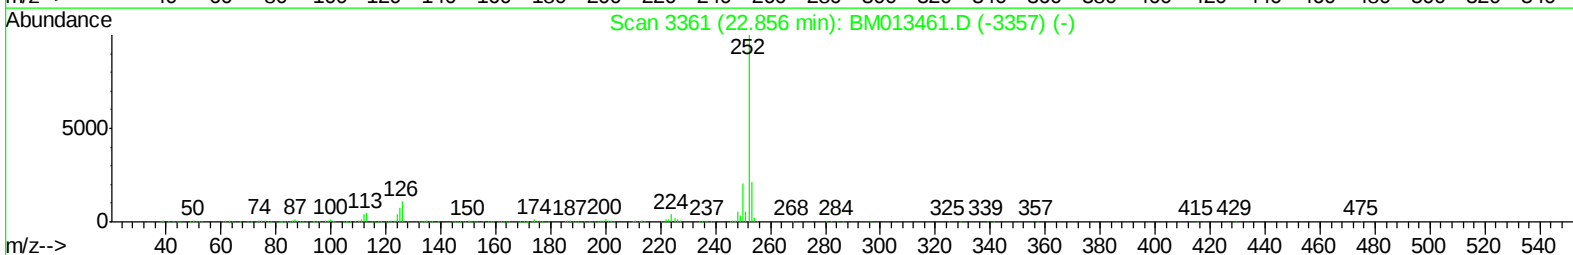
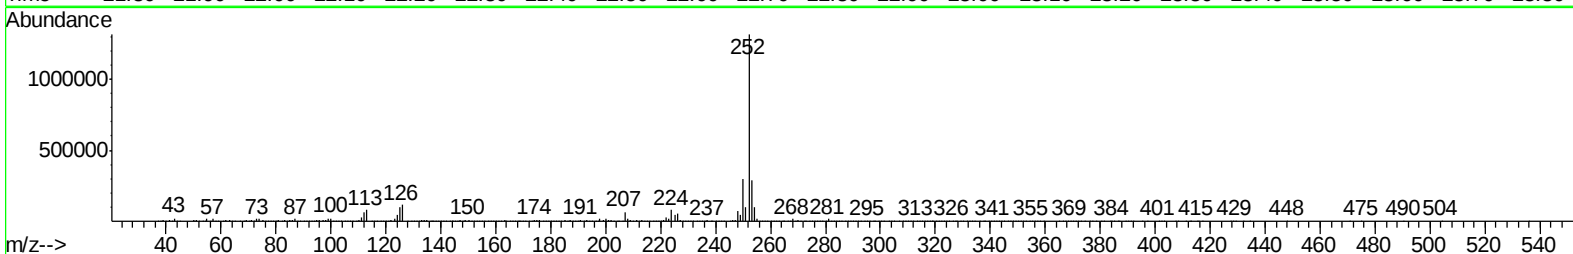


Data File : BM013475.D
Acq On : 16 Dec 2017 12:58
Operator : SJ/JU
Sample : I6799-06
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Dec 18 00:31:11 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

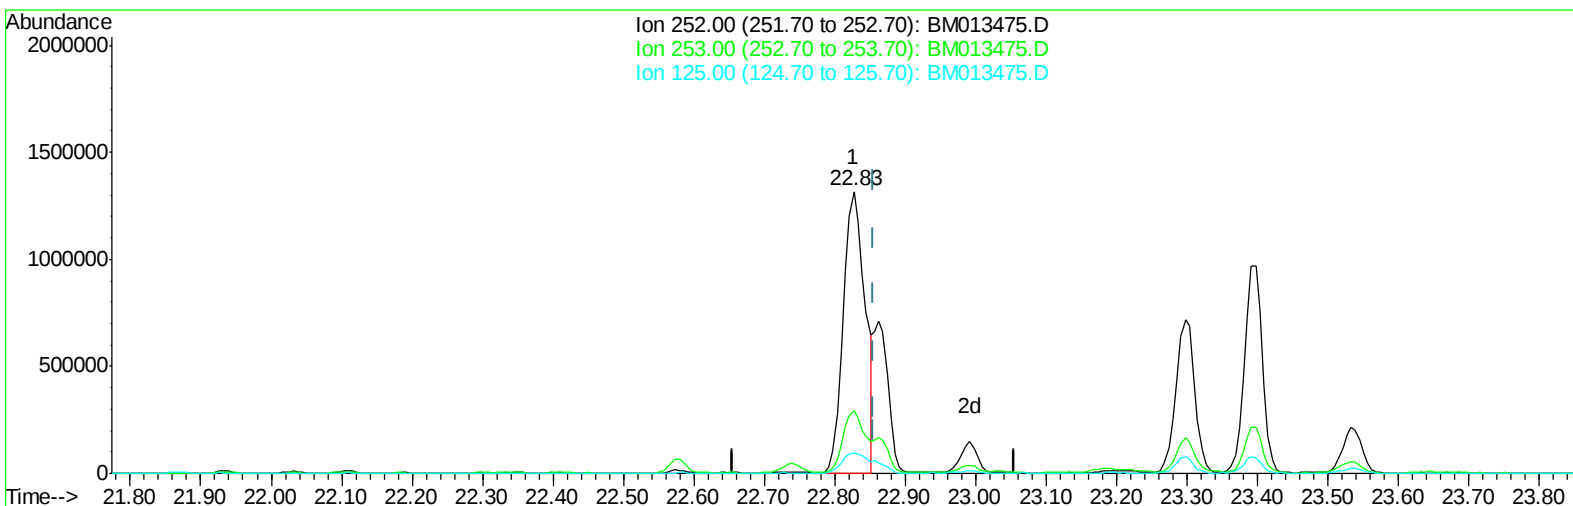

TIC: BM013475.D

(86) Benzo(k)fluoranthene

22.827min (-0.030) 43.98ng/ul

response 2801607

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.26
125.00	4.30	7.30#
0.00	0.00	0.00