
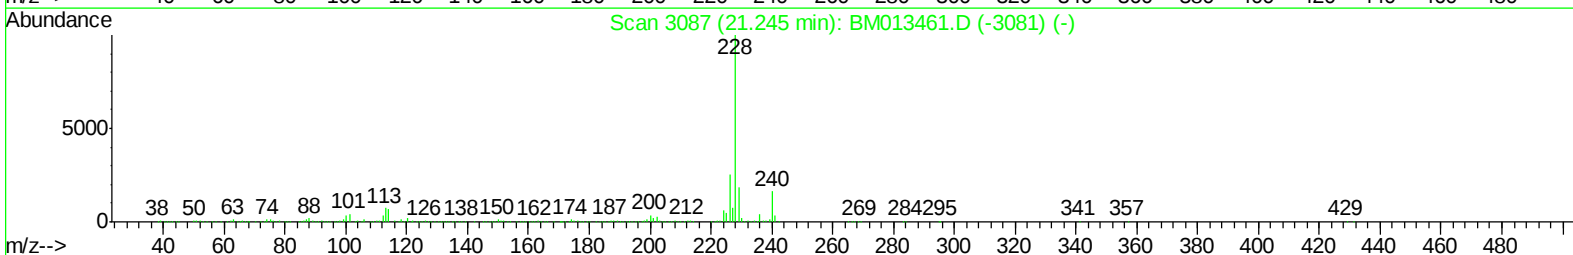
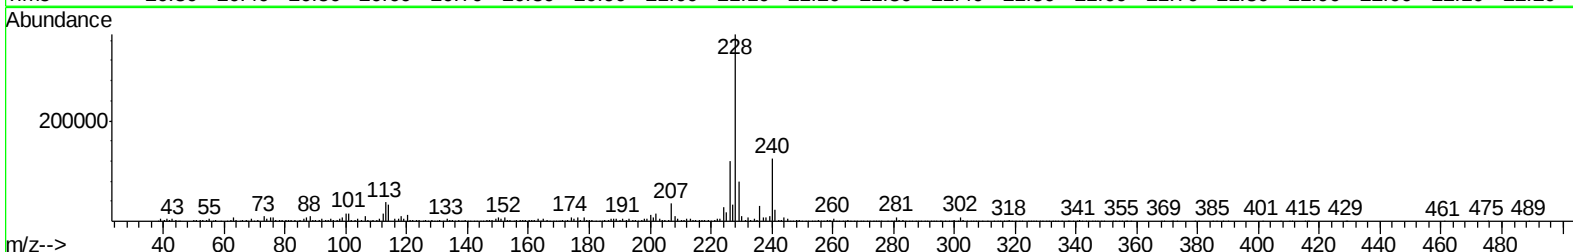


Data File : BM013476.D
Acq On : 16 Dec 2017 13:34
Operator : SJ/JU
Sample : I6779-11
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 00:31:31 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

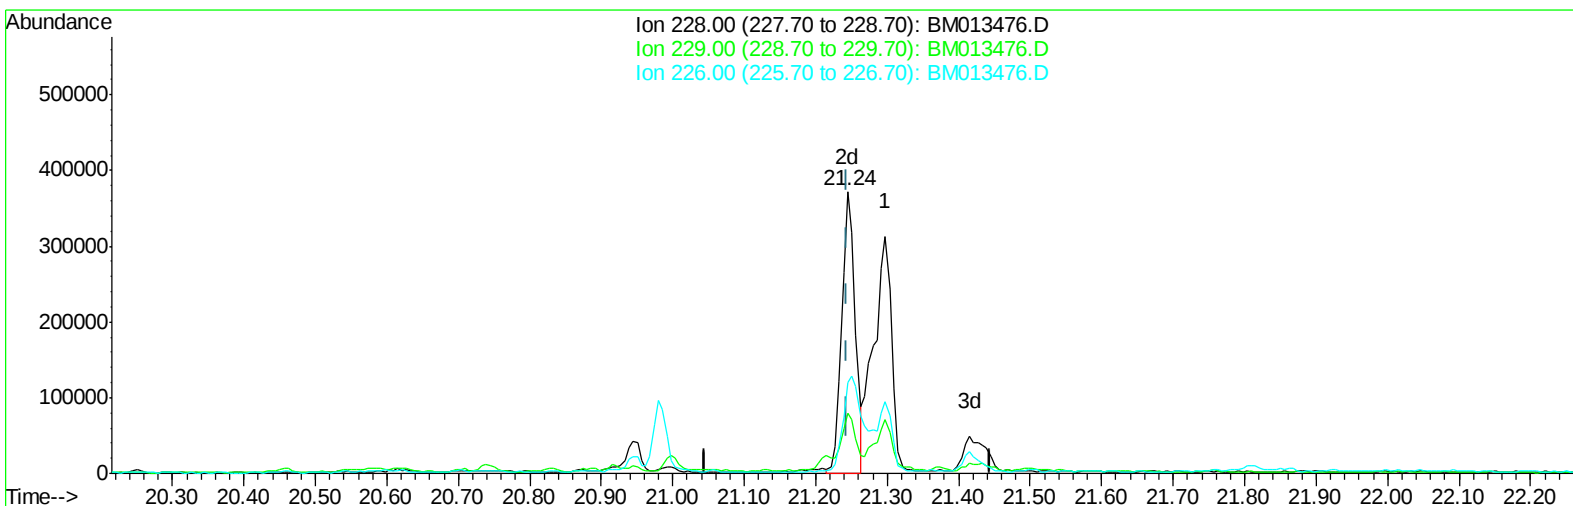

TIC: BM013476.D

(80) Benzo(a)anthracene
21.245min (-0.000) 6.93ng/ul m
response 491100

Ion	Exp%	Act%
228.00	100	100
229.00	19.20	21.22
226.00	26.70	32.12#
0.00	0.00	0.00