
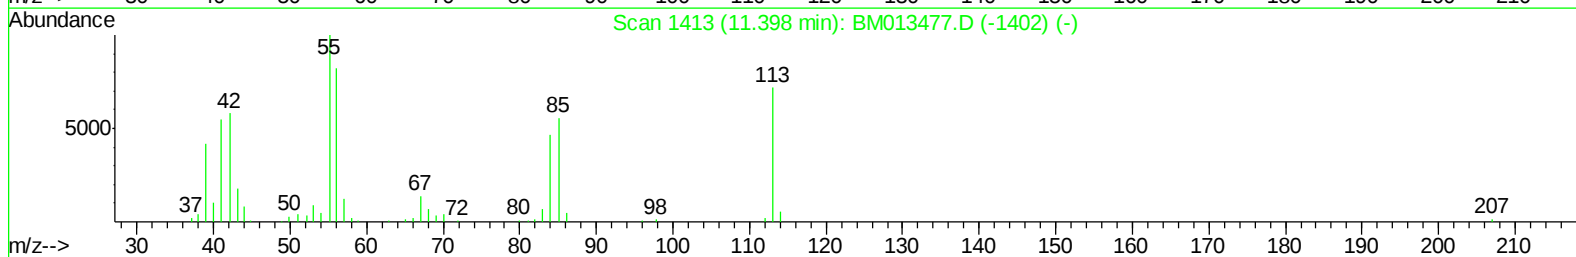
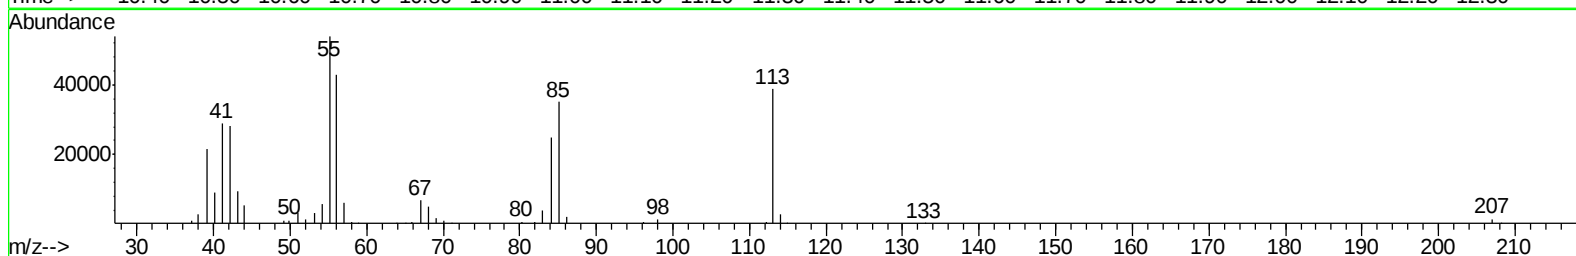


Data File : BM013488.D
Acq On : 16 Dec 2017 21:55
Operator : SJ/JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Dec 18 03:16:19 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 18 03:13:05 2017
Response via : Initial Calibration

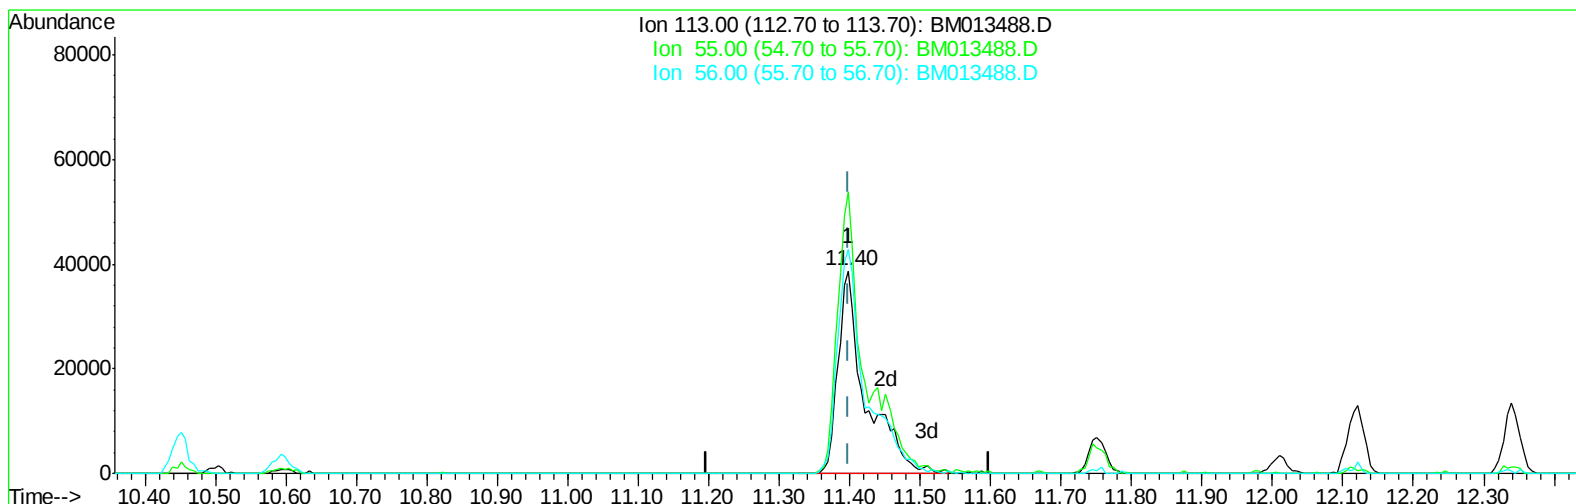

TIC: BM013488.D

(32) Caprolactam

11.398min (+0.000) 19.49ng/ul m

response 105464

Ion	Exp%	Act%
113.00	100	100
55.00	260.00	138.91#
56.00	200.00	110.44#
0.00	0.00	0.00