
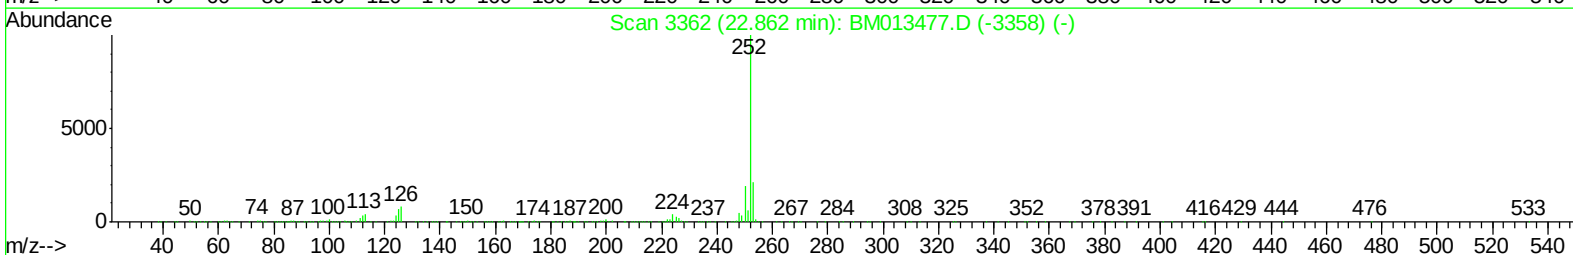
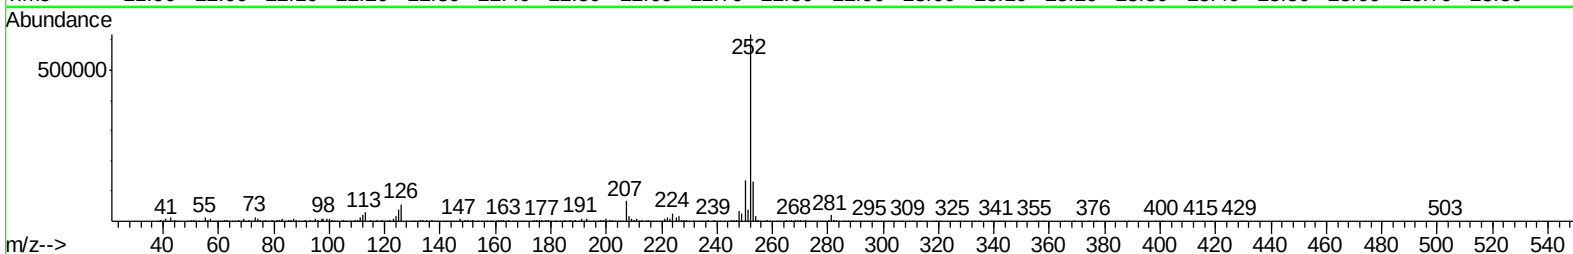


Data File : BM013480.D
Acq On : 16 Dec 2017 17:10
Operator : SJ/JU
Sample : I6776-14
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Dec 18 03:13:36 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 18 03:13:05 2017
Response via : Initial Calibration

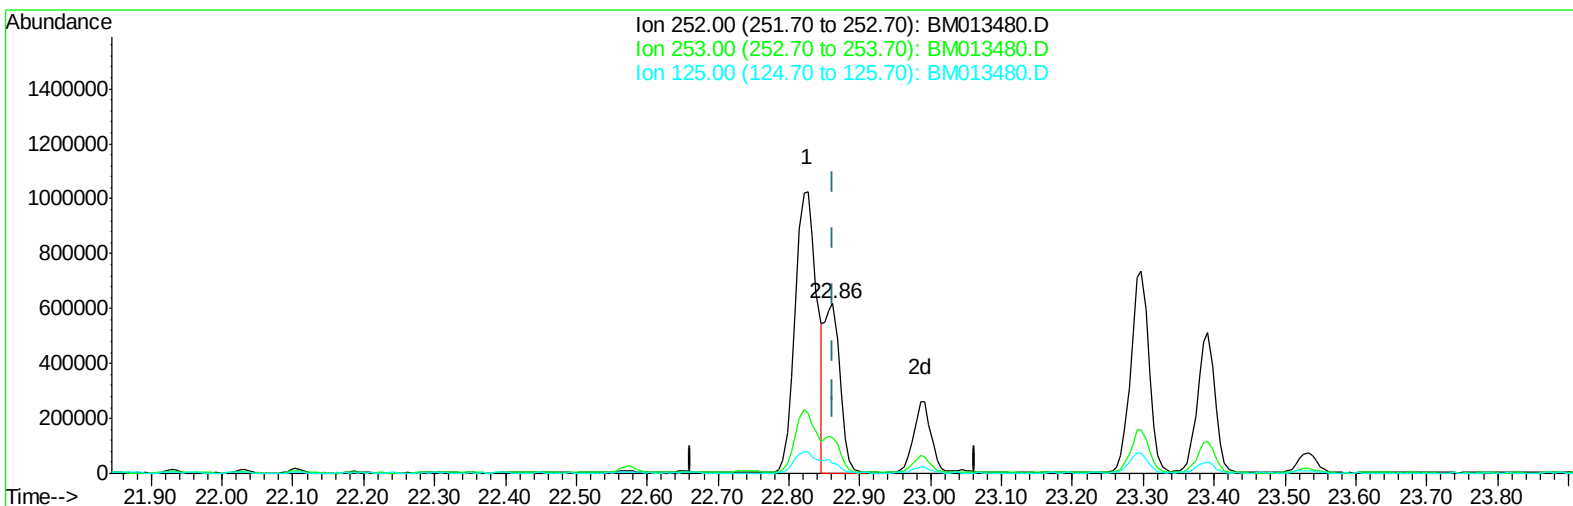

TIC: BM013480.D

(86) Benzo(k)fluoranthene

22.862min (-0.000) 18.52ng/ul m

response 969520

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	21.14
125.00	4.30	6.25#
0.00	0.00	0.00