
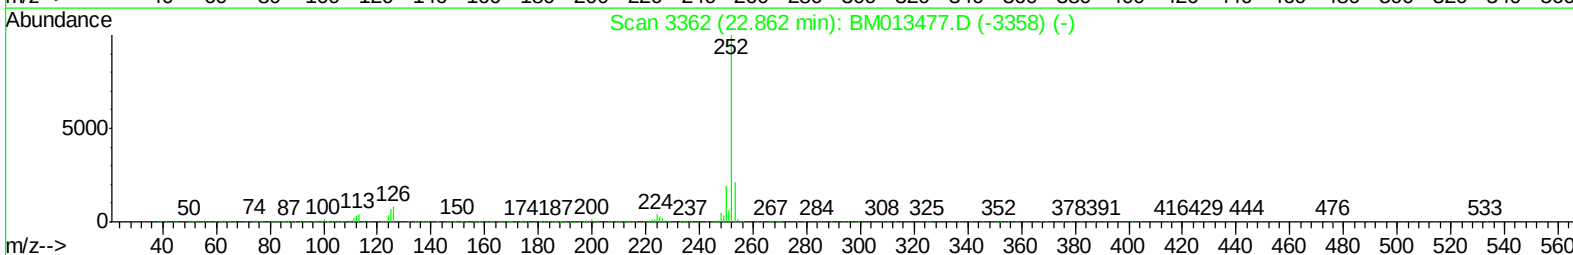
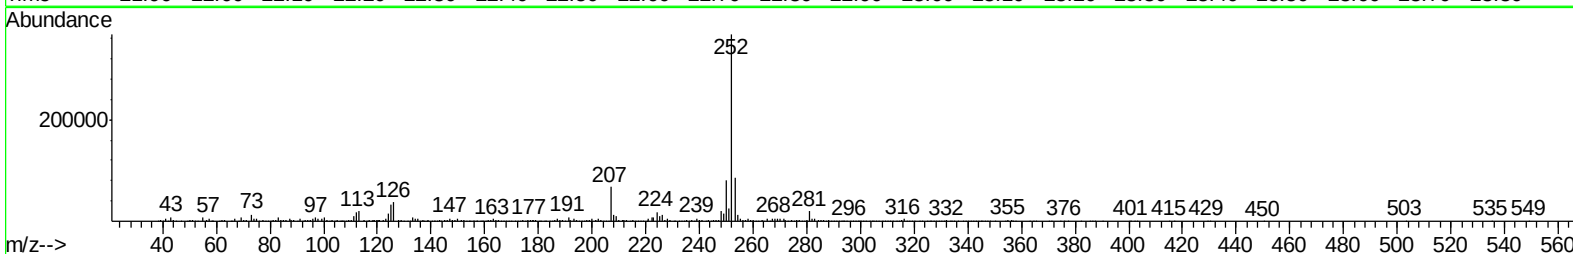


Data File : BM013481.D
Acq On : 16 Dec 2017 17:46
Operator : SJ/JU
Sample : I6778-10
Misc :
ALS Vial : 38 Sample Multiplier: 1

Quant Time: Dec 18 03:13:54 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 18 03:13:05 2017
Response via : Initial Calibration

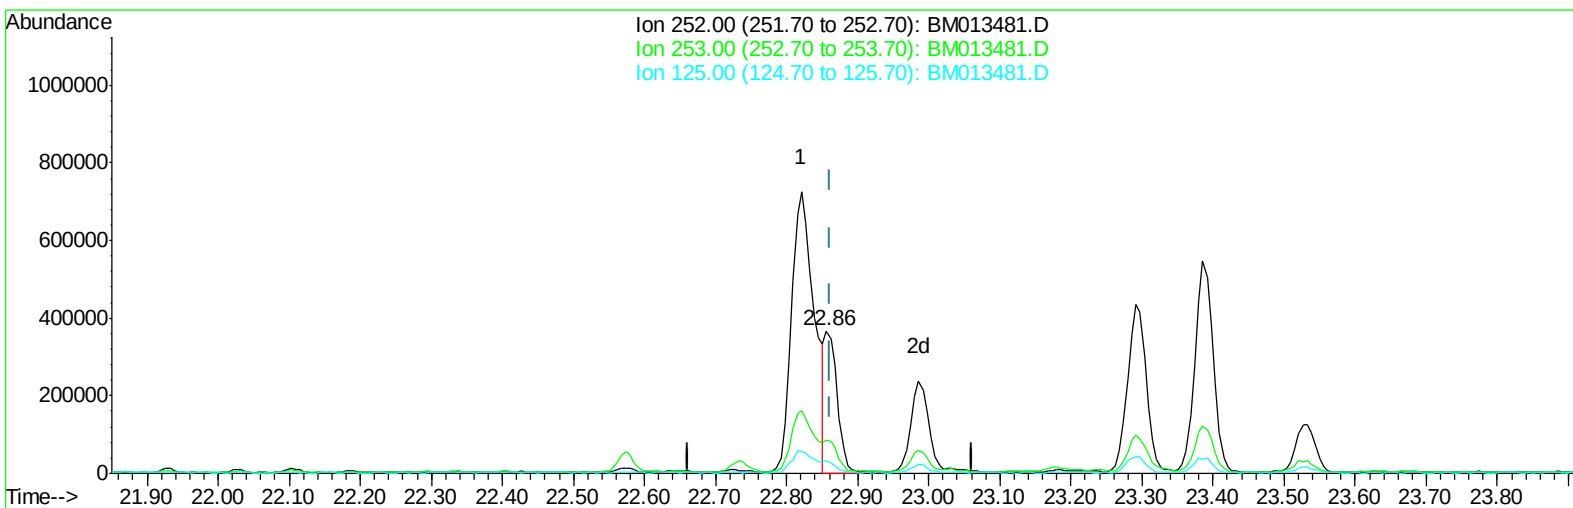

TIC: BM013481.D

(86) Benzo(k)fluoranthene

22.856min (-0.006) 8.20ng/ul m

response 437037

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	23.71
125.00	4.30	8.79#
0.00	0.00	0.00