
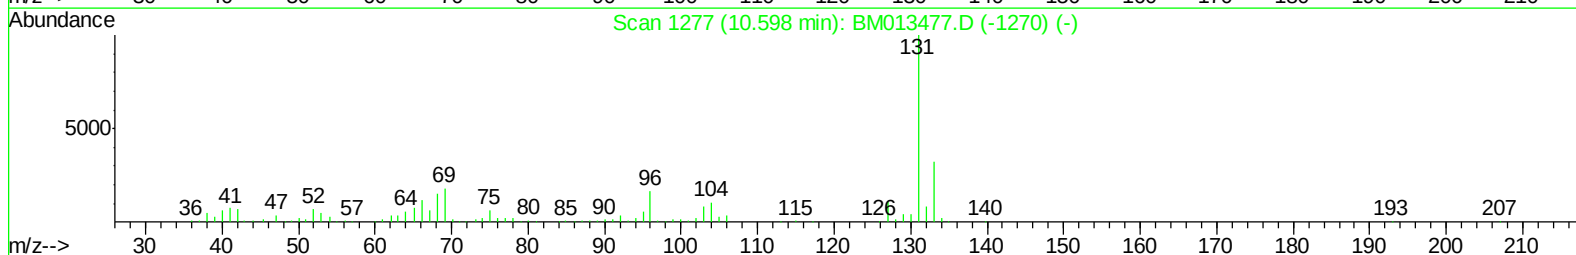
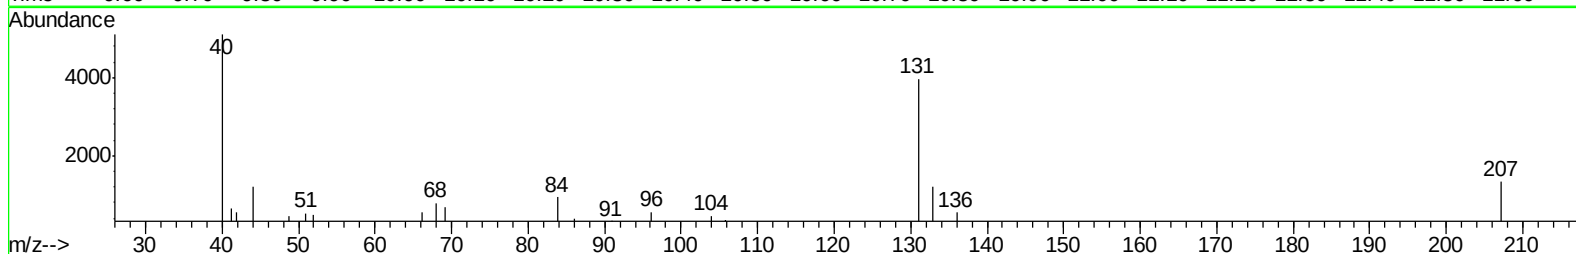


Data File : BM013483.D
Acq On : 16 Dec 2017 18:58
Operator : SJ/JU
Sample : I6775-10DL 30X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 18 03:14:39 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 18 03:13:05 2017
Response via : Initial Calibration

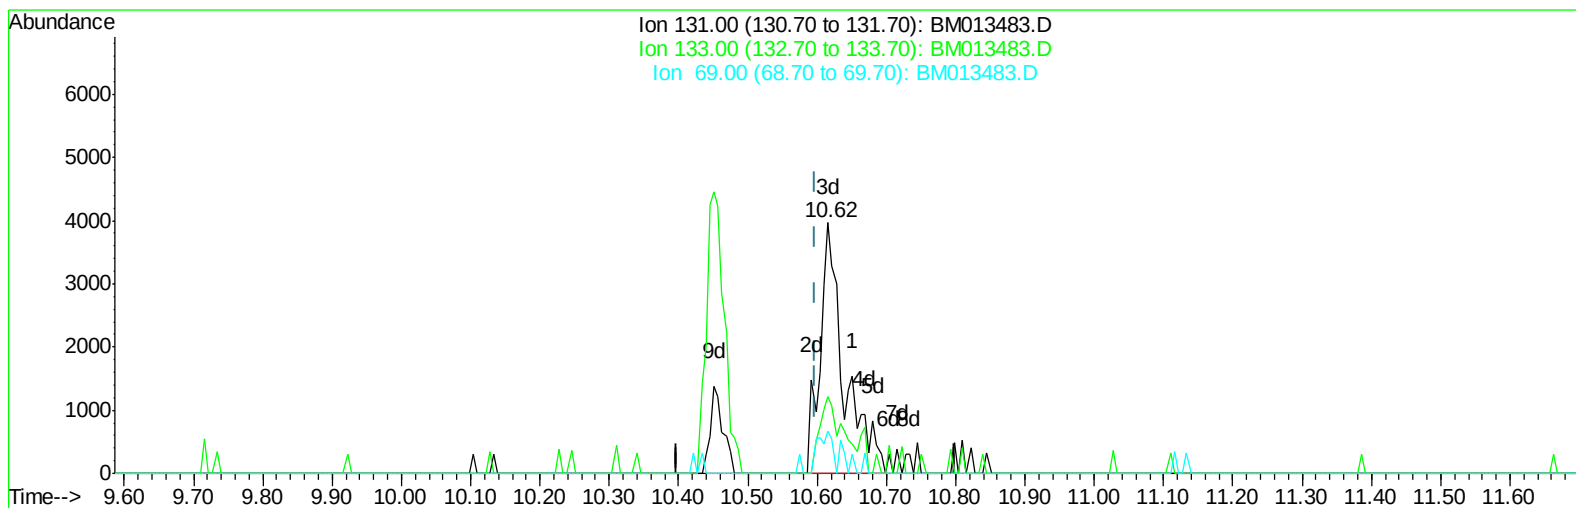

TIC: BM013483.D

(29) 4-Chloroaniline-d4 (S)

10.616min (+0.017) 0.54ng/ul m

response 9494

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	30.49
69.00	24.30	16.95#
0.00	0.00	0.00