
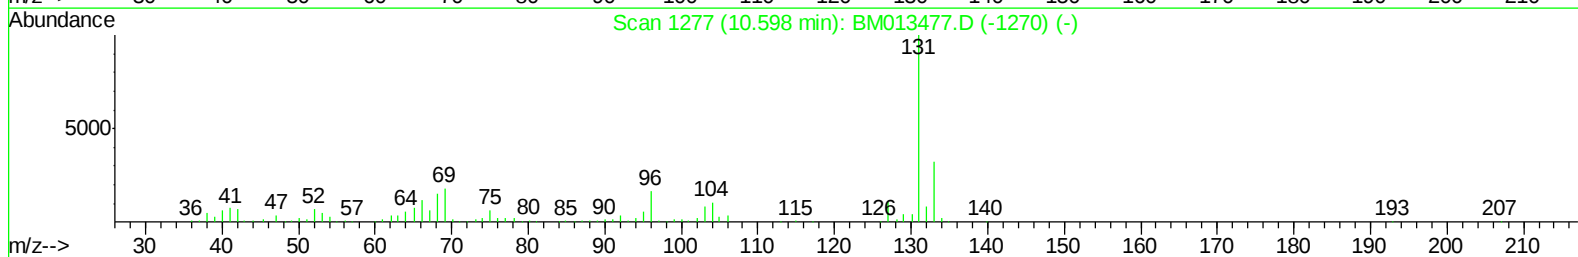
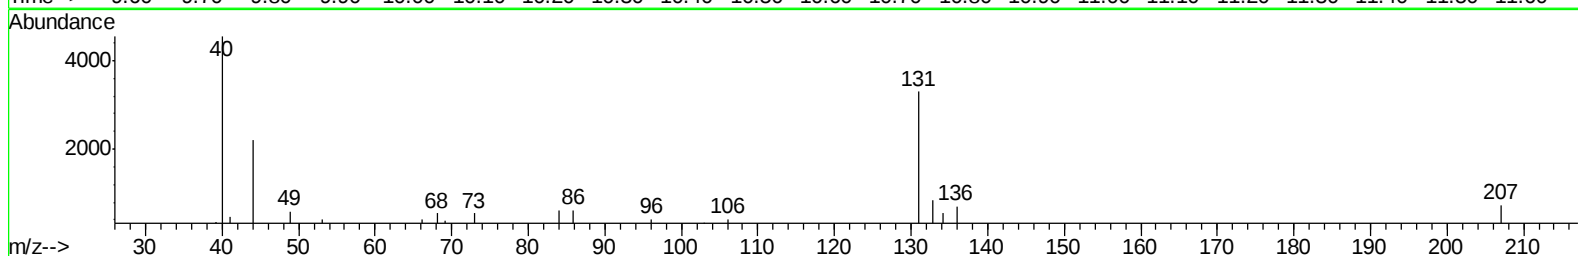


Data File : BM013484.D  
Acq On : 16 Dec 2017 19:33  
Operator : SJ/JU  
Sample : I6776-17DL 25X  
Misc :  
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Dec 18 03:14:52 2017  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM113017.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Mon Dec 18 03:13:05 2017  
Response via : Initial Calibration

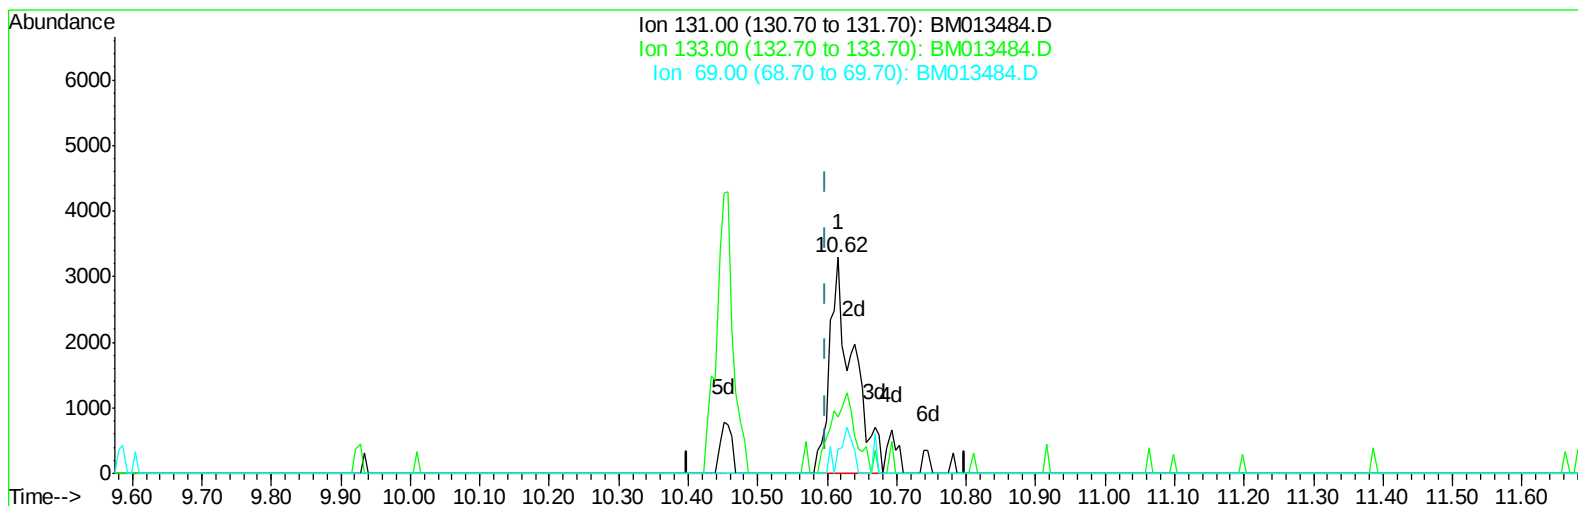

TIC: BM013484.D

(29) 4-Chloroaniline-d4 (S)

10.616min (+0.017) 0.54ng/ul m

response 7883

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 131.00 | 100   | 100    |
| 133.00 | 31.40 | 25.92  |
| 69.00  | 24.30 | 11.58# |
| 0.00   | 0.00  | 0.00   |