
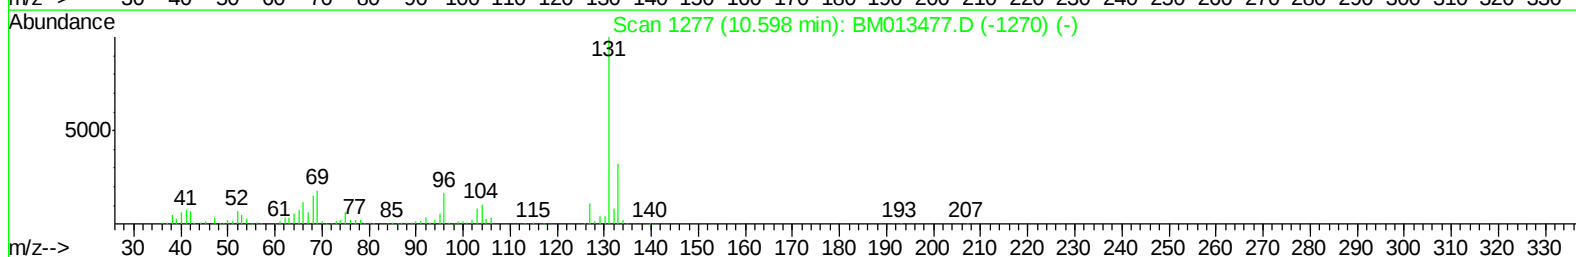
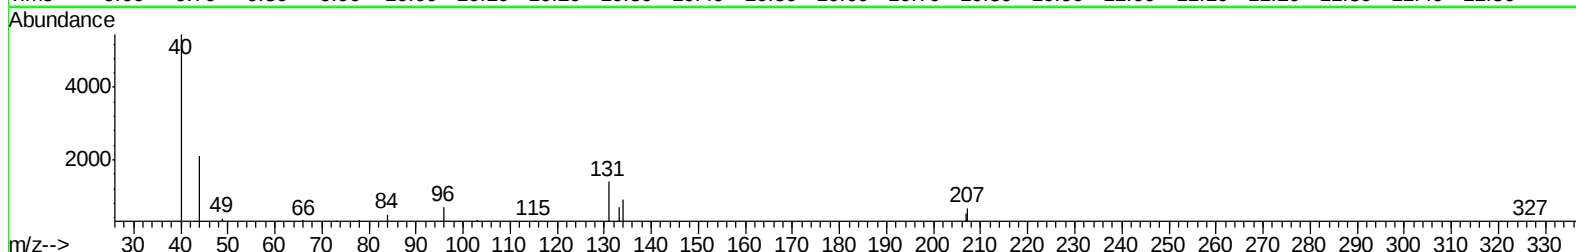


Data File : BM013485.D
Acq On : 16 Dec 2017 20:09
Operator : SJ/JU
Sample : I6776-18DL 20X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Quant Time: Dec 18 03:15:10 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 18 03:13:05 2017
Response via : Initial Calibration

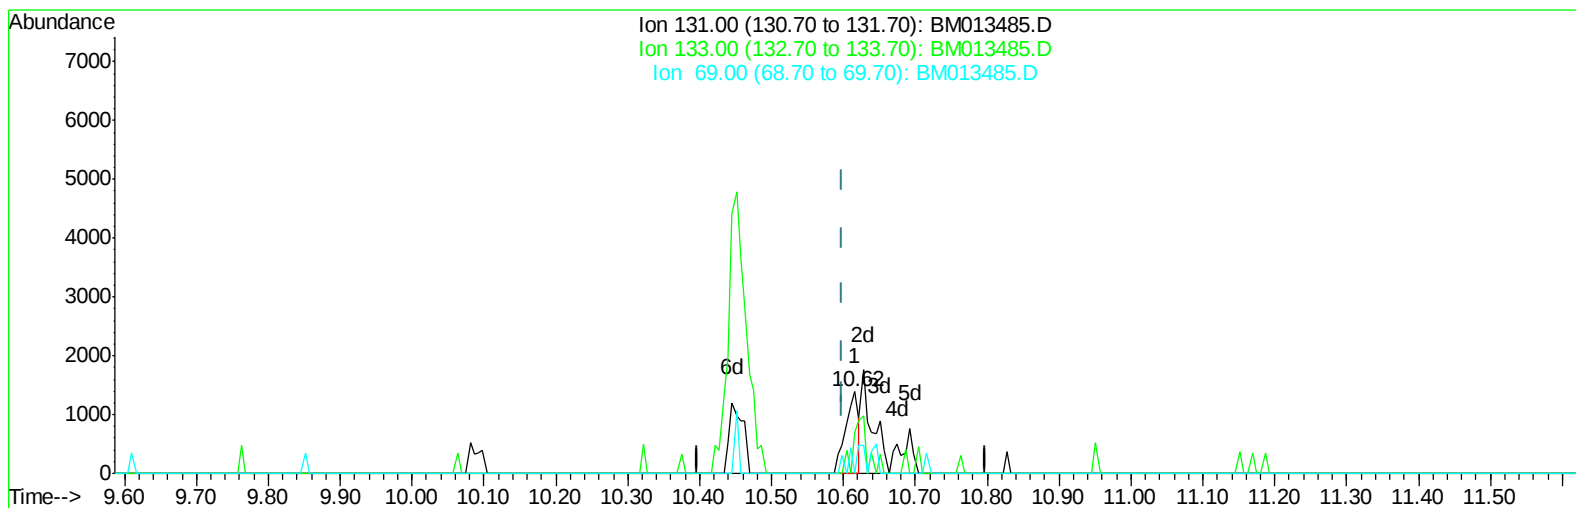

TIC: BM013485.D

(29) 4-Chloroaniline-d4 (S)
10.616min (+0.018) 0.12ng/ul
response 1822

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	49.89#
69.00	24.30	0.00#
0.00	0.00	0.00