
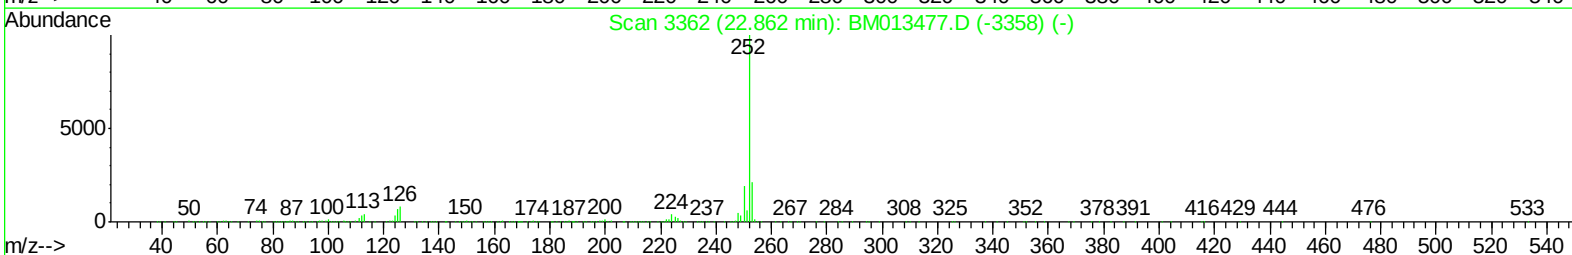
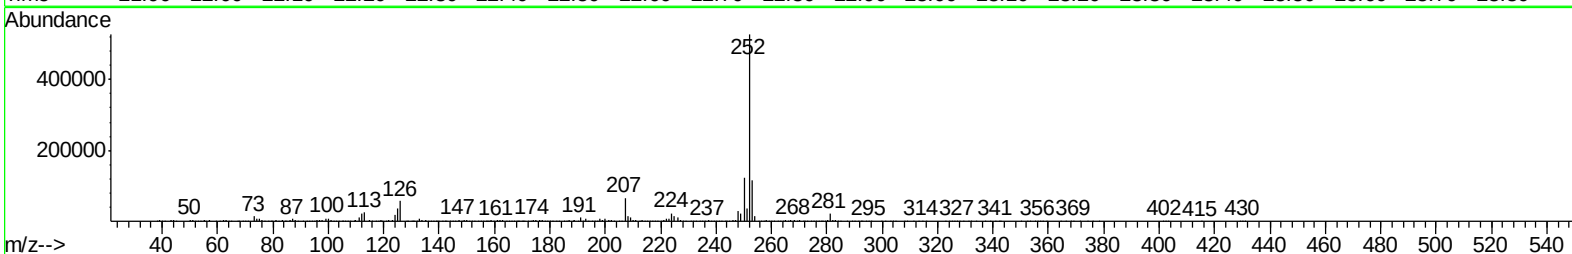


Data File : BM013485.D
Acq On : 16 Dec 2017 20:09
Operator : SJ/JU
Sample : I6776-18DL 20X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Quant Time: Dec 18 03:15:10 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 18 03:13:05 2017
Response via : Initial Calibration

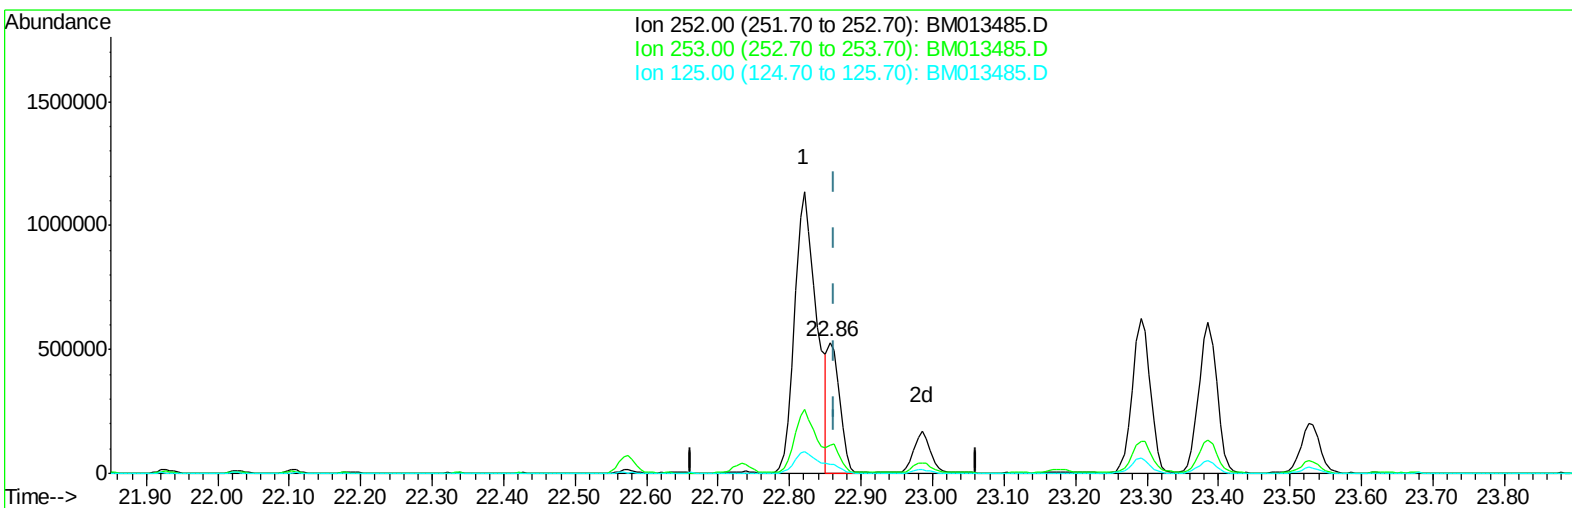

TIC: BM013485.D

(86) Benzo(k)fluoranthene

22.856min (-0.006) 11.42ng/ul m

response 596885

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	21.72
125.00	4.30	7.15#
0.00	0.00	0.00