
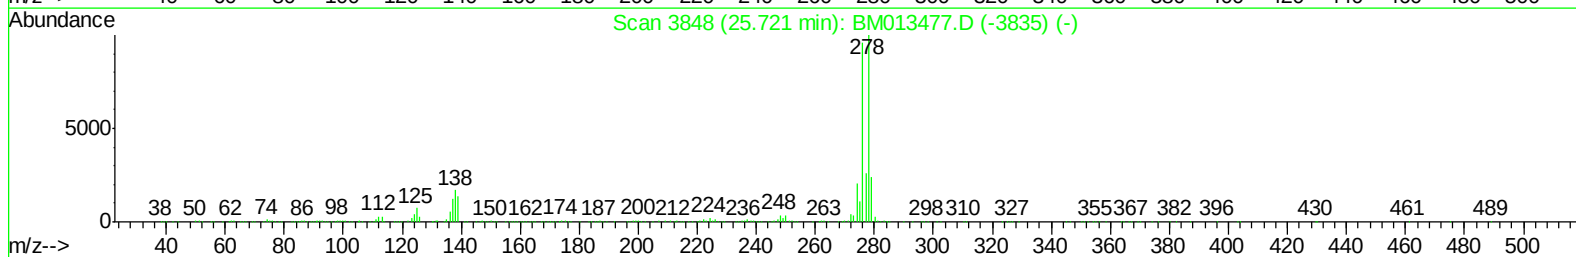
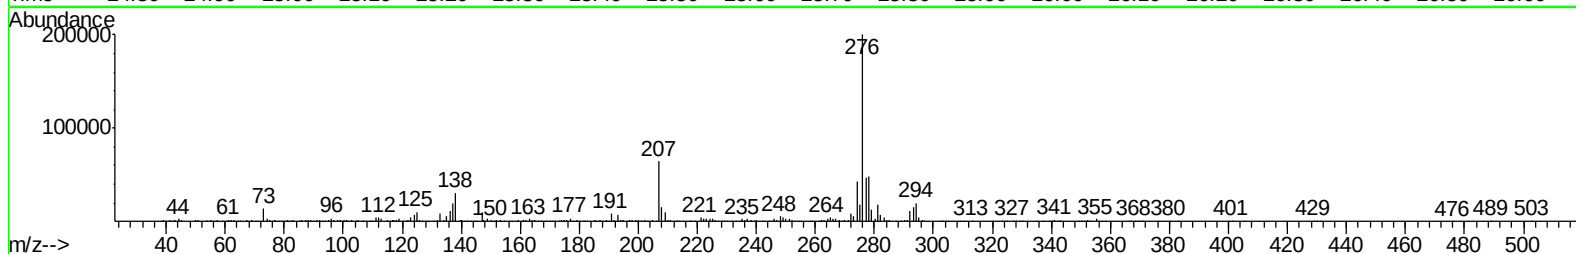


Data File : BM013485.D
Acq On : 16 Dec 2017 20:09
Operator : SJ/JU
Sample : I6776-18DL 20X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Quant Time: Dec 18 03:48:56 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 18 03:13:05 2017
Response via : Initial Calibration

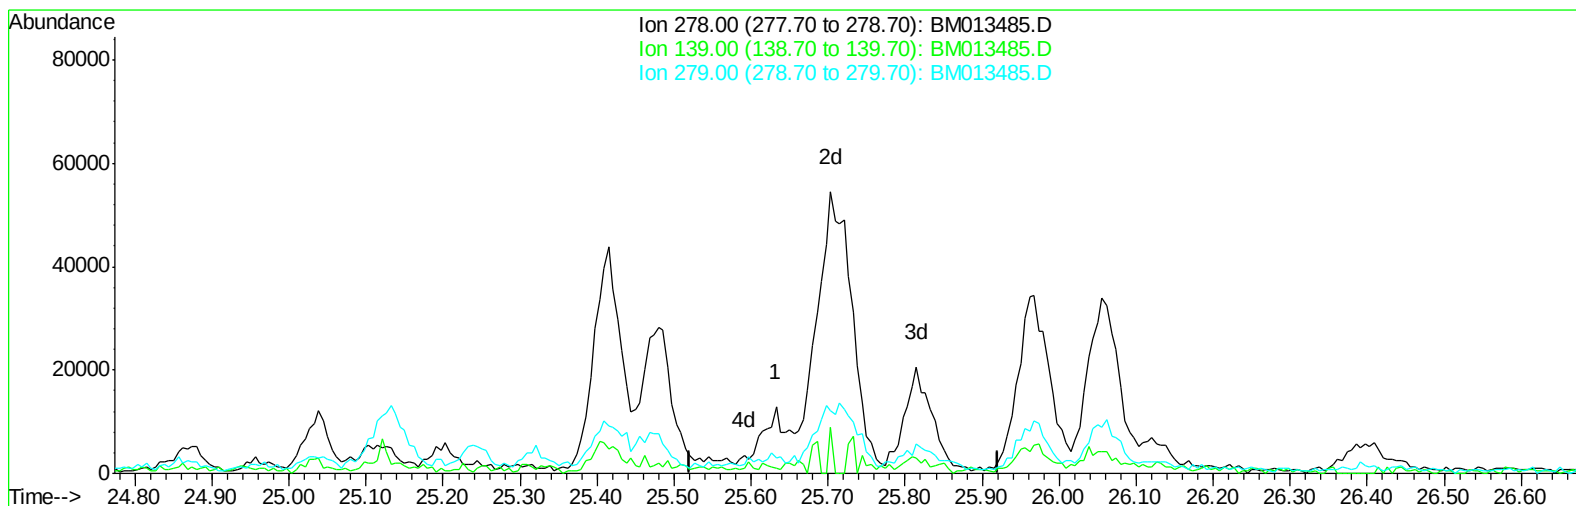

TIC: BM013485.D

(90) Dibenzo(a,h)anthracene

25.721min (-25.721) 0.00ng/ul d

response 0

Ion	Exp%	Act%
278.00	100	0.00
139.00	7.30	0.00
279.00	23.20	0.00
0.00	0.00	0.00